


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101123\
Data File : VU055736.D
Acq On : 11 Oct 2023 09:31
Operator : MD/SY
Sample : BFB021
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB021

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Title : VOC Analysis
Last Update : Thu Oct 12 01:53:31 2023

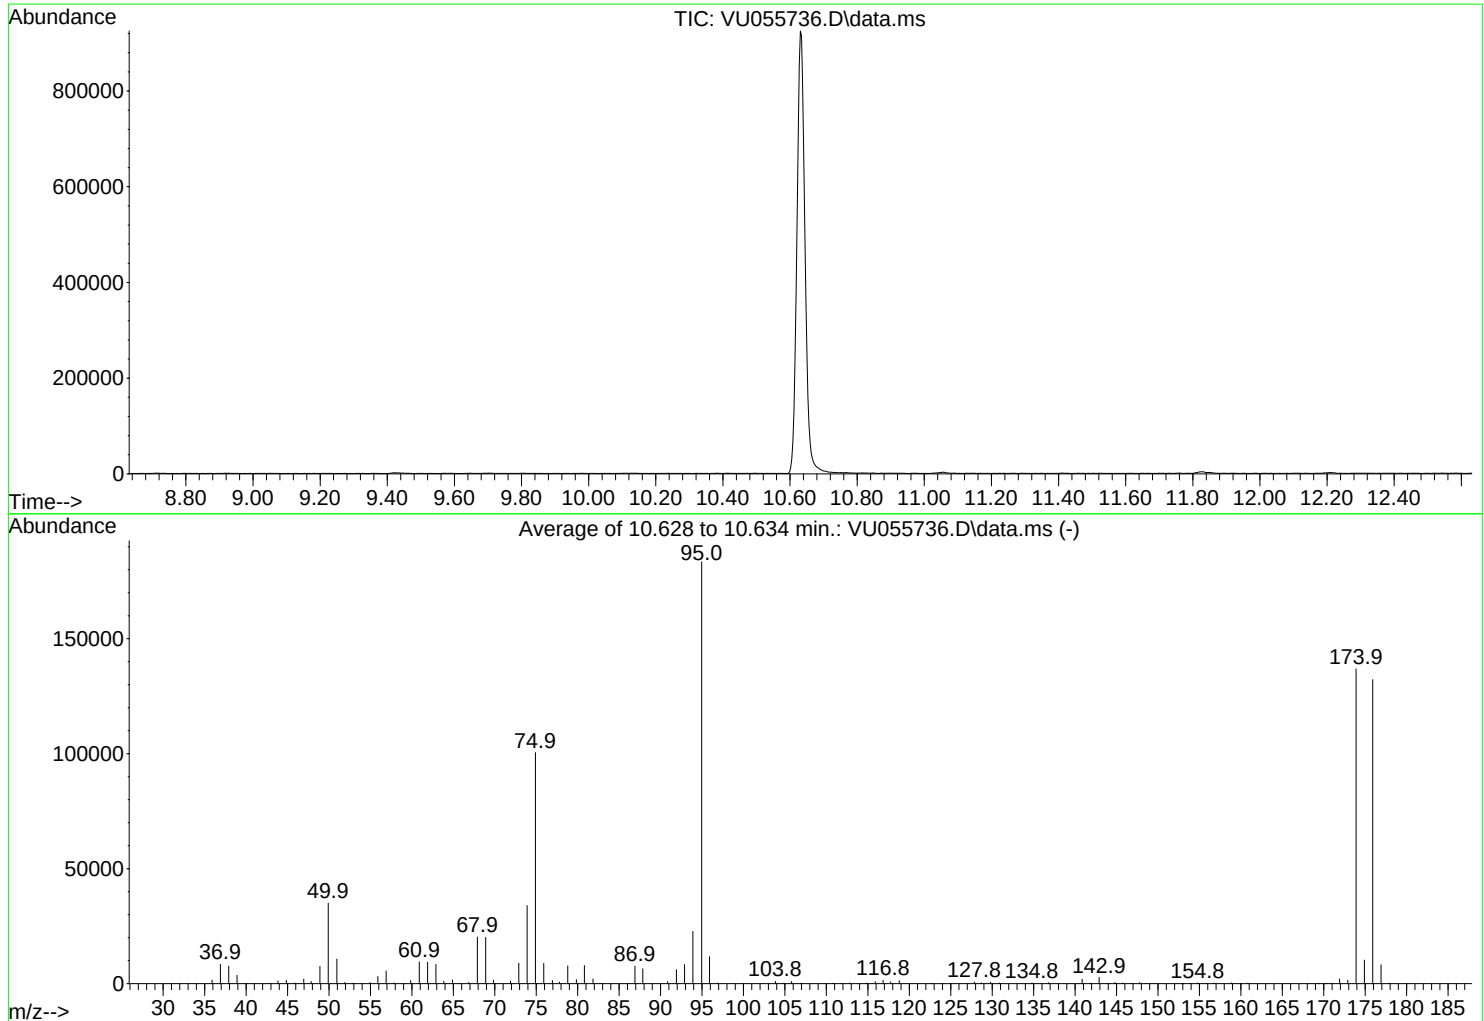

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	35003	PASS
75	95	30	80	54.8	100525	PASS
95	95	100	100	100.0	183445	PASS
96	95	5	9	6.4	11700	PASS
173	174	0.00	2	1.1	1481	PASS
174	95	50	120	74.6	136883	PASS
175	174	5	9	7.5	10242	PASS
176	174	95	101	96.6	132237	PASS
177	176	5	9	6.2	8211	PASS

m/z	Abundance
39.80	332.0
43.80	403.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021

m/z	Abundance
35.90	1430.0
36.90	8170.0
37.90	7724.0
38.90	3430.0
39.90	561.0
41.00	178.0
42.80	176.0
43.90	1603.0
44.80	1309.0
45.80	220.0
46.90	1876.0
47.90	862.0
48.90	7550.0
49.90	33632.0
51.00	10453.0
51.90	431.0
52.90	223.0
54.00	112.0
55.00	413.0
55.90	3066.0
56.90	5378.0
57.90	251.0
59.90	1370.0
60.90	9152.0
61.90	9149.0
62.90	8007.0
63.80	1074.0
64.90	1453.0
65.90	139.0
66.90	583.0
67.90	19736.0
68.90	19632.0
69.90	1423.0
71.90	1109.0
72.90	8894.0
73.90	32552.0
74.90	96584.0
75.90	8712.0
77.00	1285.0
77.70	622.0
78.80	7534.0
79.90	1711.0
80.80	7345.0
81.80	1978.0
82.70	130.0
86.90	7395.0
87.80	5991.0
90.80	794.0
91.90	5460.0
92.90	8151.0
93.90	22232.0
94.90	174272.0
95.90	11198.0
96.90	319.0
103.90	898.0
104.80	215.0
105.80	955.0
106.90	209.0
110.80	200.0
111.70	120.0
112.80	251.0
114.80	276.0
115.90	829.0
116.90	1427.0
117.80	680.0
118.80	1189.0
122.70	112.0
127.90	614.0
128.70	281.0
129.80	604.0
130.90	241.0
134.80	304.0
136.80	392.0
140.80	1980.0
141.90	214.0
142.90	2412.0
143.80	136.0
144.80	544.0
145.70	330.0
146.70	120.0
147.80	466.0
148.60	125.0
149.60	145.0
153.80	135.0
154.80	340.0
155.80	121.0
156.70	324.0
158.90	399.0
160.90	247.0
171.00	233.0
171.90	1833.0
172.90	1210.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021

173.90	128088.0
174.90	9711.0
175.90	123496.0
176.90	7852.0
177.80	239.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021

m/z	Abundance
35.90	1647.0
36.90	8655.0
37.90	7726.0
38.90	3704.0
39.90	483.0
41.00	136.0
42.80	144.0
43.90	1654.0
44.80	1532.0
45.80	293.0
46.90	2015.0
47.90	1005.0
48.90	7624.0
49.90	36176.0
50.90	11141.0
51.90	490.0
52.90	196.0
53.90	115.0
54.90	465.0
55.90	3209.0
56.90	5729.0
57.80	266.0
59.90	1283.0
60.90	9800.0
61.90	9623.0
62.90	8690.0
63.80	1116.0
64.90	1674.0
65.90	196.0
66.80	571.0
67.90	20976.0
68.90	20472.0
69.80	1545.0
71.90	1196.0
72.90	9289.0
73.90	34944.0
74.90	103728.0
75.90	8983.0
76.90	1439.0
77.80	695.0
78.80	8021.0
79.90	1715.0
80.80	8136.0
81.90	2133.0
82.70	112.0
86.90	7787.0
87.80	6562.0
90.80	851.0
91.90	6224.0
92.90	8523.0
93.90	23328.0
95.00	189376.0
95.90	12018.0
96.90	285.0
103.90	970.0
104.80	214.0
105.80	950.0
106.90	264.0
110.80	247.0
111.80	137.0
112.80	300.0
114.80	302.0
115.90	902.0
116.80	1494.0
117.70	770.0
118.80	1370.0
123.90	120.0
127.80	772.0
128.70	349.0
129.80	622.0
130.80	277.0
134.80	322.0
136.80	421.0
140.80	2009.0
141.80	222.0
142.90	2867.0
143.80	153.0
144.80	508.0
145.80	339.0
146.80	140.0
147.80	531.0
149.00	140.0
149.60	150.0
153.80	142.0
154.80	378.0
155.80	158.0
156.80	312.0
158.90	363.0
160.80	316.0
170.70	174.0
171.00	194.0
171.90	2047.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021

172.90	1526.0
173.90	140800.0
174.90	10629.0
175.90	136064.0
176.90	8380.0
177.90	240.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021

m/z	Abundance
35.90	1647.0
36.90	8286.0
37.90	7299.0
38.90	3702.0
40.00	501.0
42.90	138.0
43.90	1604.0
44.90	1565.0
45.80	313.0
47.00	2065.0
47.80	1068.0
48.90	7401.0
49.90	35200.0
50.90	10671.0
51.90	498.0
52.90	196.0
53.80	128.0
54.90	506.0
55.90	3119.0
56.90	5429.0
57.80	238.0
59.80	1409.0
60.90	9520.0
61.90	9308.0
62.90	8401.0
63.90	1078.0
64.90	1733.0
65.90	196.0
66.80	555.0
67.90	20056.0
68.90	20152.0
69.80	1620.0
71.90	1132.0
72.90	8618.0
73.90	34304.0
74.90	101264.0
75.90	8651.0
76.90	1490.0
77.90	715.0
78.80	7701.0
79.80	1827.0
80.80	8166.0
81.90	1950.0
82.70	114.0
85.90	258.0
86.90	7515.0
87.90	6920.0
90.90	866.0
91.90	6413.0
92.90	8196.0
93.90	22408.0
95.00	186688.0
95.90	11884.0
96.80	295.0
103.80	1094.0
104.70	227.0
105.80	866.0
107.00	257.0
109.70	138.0
110.80	255.0
111.80	165.0
112.80	291.0
114.80	300.0
115.90	878.0
116.80	1432.0
117.70	863.0
118.80	1384.0
123.90	139.0
127.90	810.0
128.70	359.0
129.80	605.0
130.80	314.0
134.80	329.0
136.80	425.0
140.90	1949.0
141.80	199.0
142.90	2860.0
143.80	121.0
144.80	439.0
145.70	263.0
146.80	136.0
147.80	526.0
149.00	193.0
149.60	114.0
152.80	116.0
153.00	113.0
153.90	123.0
154.80	355.0
155.80	142.0
156.80	313.0
158.80	275.0
160.80	325.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021

169.40	117.0
170.20	100.0
170.70	114.0
171.10	136.0
171.90	2110.0
172.90	1706.0
173.90	141760.0
174.90	10387.0
175.90	137152.0
176.90	8400.0
177.90	202.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021