

Data File : VU027614.D
Acq On : 12 Oct 2018 10:01
Operator : MD/SY
Sample : J5403-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0906

Quant Time: Oct 22 07:07:59 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 13 01:37:08 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	183995	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	168677	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	69391	50.00	ug/L	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) Vinyl Chloride-d3	1.40	65	64704	44.69	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	89.38%		
7) Chloroethane-d5	1.68	69	51411	46.09	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	92.18%		
11) 1,1-Dichloroethene-d2	2.28	63	91721	33.77	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	67.54%		
21) 2-Butanone-d5	4.18	46	106152	90.81	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	90.81%		
24) Chloroform-d	4.65	84	108424	46.82	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.64%		
26) 1,2-Dichloroethane-d4	5.31	65	75330	46.41	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.82%		
32) Benzene-d6	5.34	84	227534	47.07	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.14%		
36) 1,2-Dichloropropane-d6	6.33	67	80804	48.80	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.60%		
41) Toluene-d8	7.57	98	190384	44.06	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.12%		
43) trans-1,3-Dichloropropene-	7.85	79	33512	42.00	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.00%		
47) 2-Hexanone-d5	8.31	63	74126	88.63	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	88.63%		
57) 1,1,2,2-Tetrachloroethane-	10.43	84	98195	45.35	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	90.70%		
64) 1,2-Dichlorobenzene-d4	11.86	152	65642	48.35	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.70%		


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	2.32	43	29531	30.801	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU027614.D
Acq On : 12 Oct 2018 10:01
Operator : MD/SY
Sample : J5403-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0906

Quant Time: Oct 22 07:07:59 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 13 01:37:08 2018
Response via : Initial Calibration

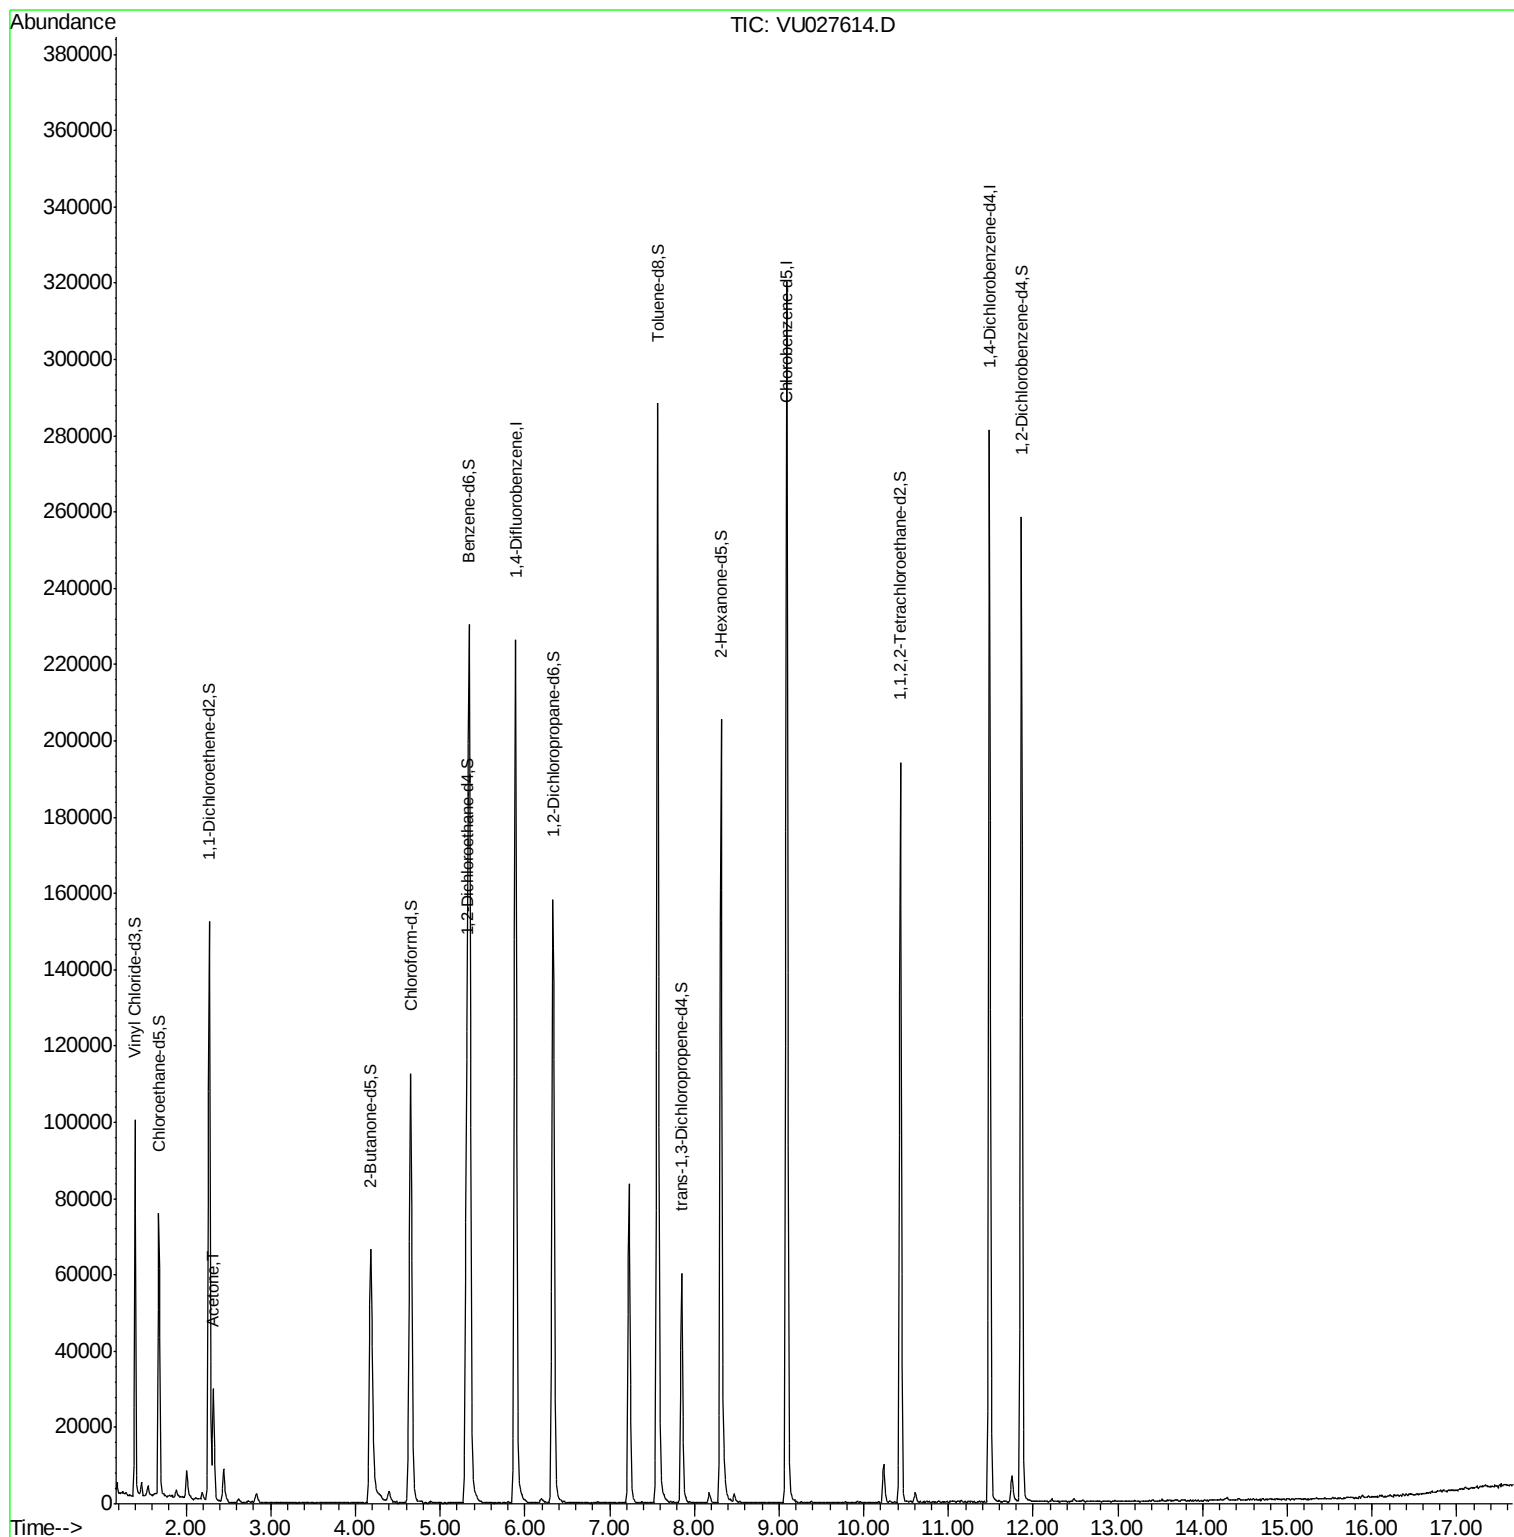

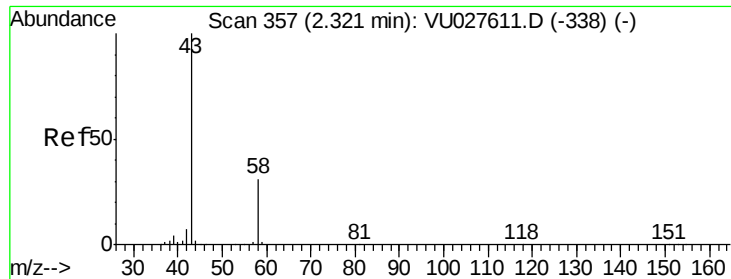

#13

Acetone

Concen: 30.801 ug/L

RT: 2.32 min Scan# 358

Delta R.T. 0.00 min

Lab File: VU027614.D

Acq: 12 Oct 2018 10:01

Instrument :

MSVOA_U

ClientSampleId :

C0906

Tgt Ion: 43 Resp: 29531

Ion Ratio Lower Upper

43 100

58 30.6 0.0 60.8

