

Data File : VU027616.D
 Acq On : 12 Oct 2018 10:47
 Operator : MD/SY
 Sample : J5405-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08X7

Quant Time: Oct 22 08:55:47 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 13 01:37:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	193185	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	172682	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	71847	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	63733	41.92	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	83.84%
7) Chloroethane-d5	1.68	69	50270	42.92	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.84%
11) 1,1-Dichloroethene-d2	2.27	63	92288	32.36	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.72%
21) 2-Butanone-d5	4.18	46	109692	89.37	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.37%
24) Chloroform-d	4.65	84	108234	44.51	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.02%
26) 1,2-Dichloroethane-d4	5.31	65	74271	43.59	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.18%
32) Benzene-d6	5.34	84	224092	45.28	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.56%
36) 1,2-Dichloropropane-d6	6.33	67	78062	46.05	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	92.10%
41) Toluene-d8	7.57	98	186289	42.11	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.22%
43) trans-1,3-Dichloropropene-	7.85	79	33740	41.30	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.60%
47) 2-Hexanone-d5	8.31	63	74701	87.25	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	87.25%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	98213	44.30	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.60%
64) 1,2-Dichlorobenzene-d4	11.86	152	65423	46.54	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.08%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	2.32	43	32530	32.315	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU027616.D
Acq On : 12 Oct 2018 10:47
Operator : MD/SY
Sample : J5405-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
C08X7

Quant Time: Oct 22 08:55:47 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 13 01:37:08 2018
Response via : Initial Calibration

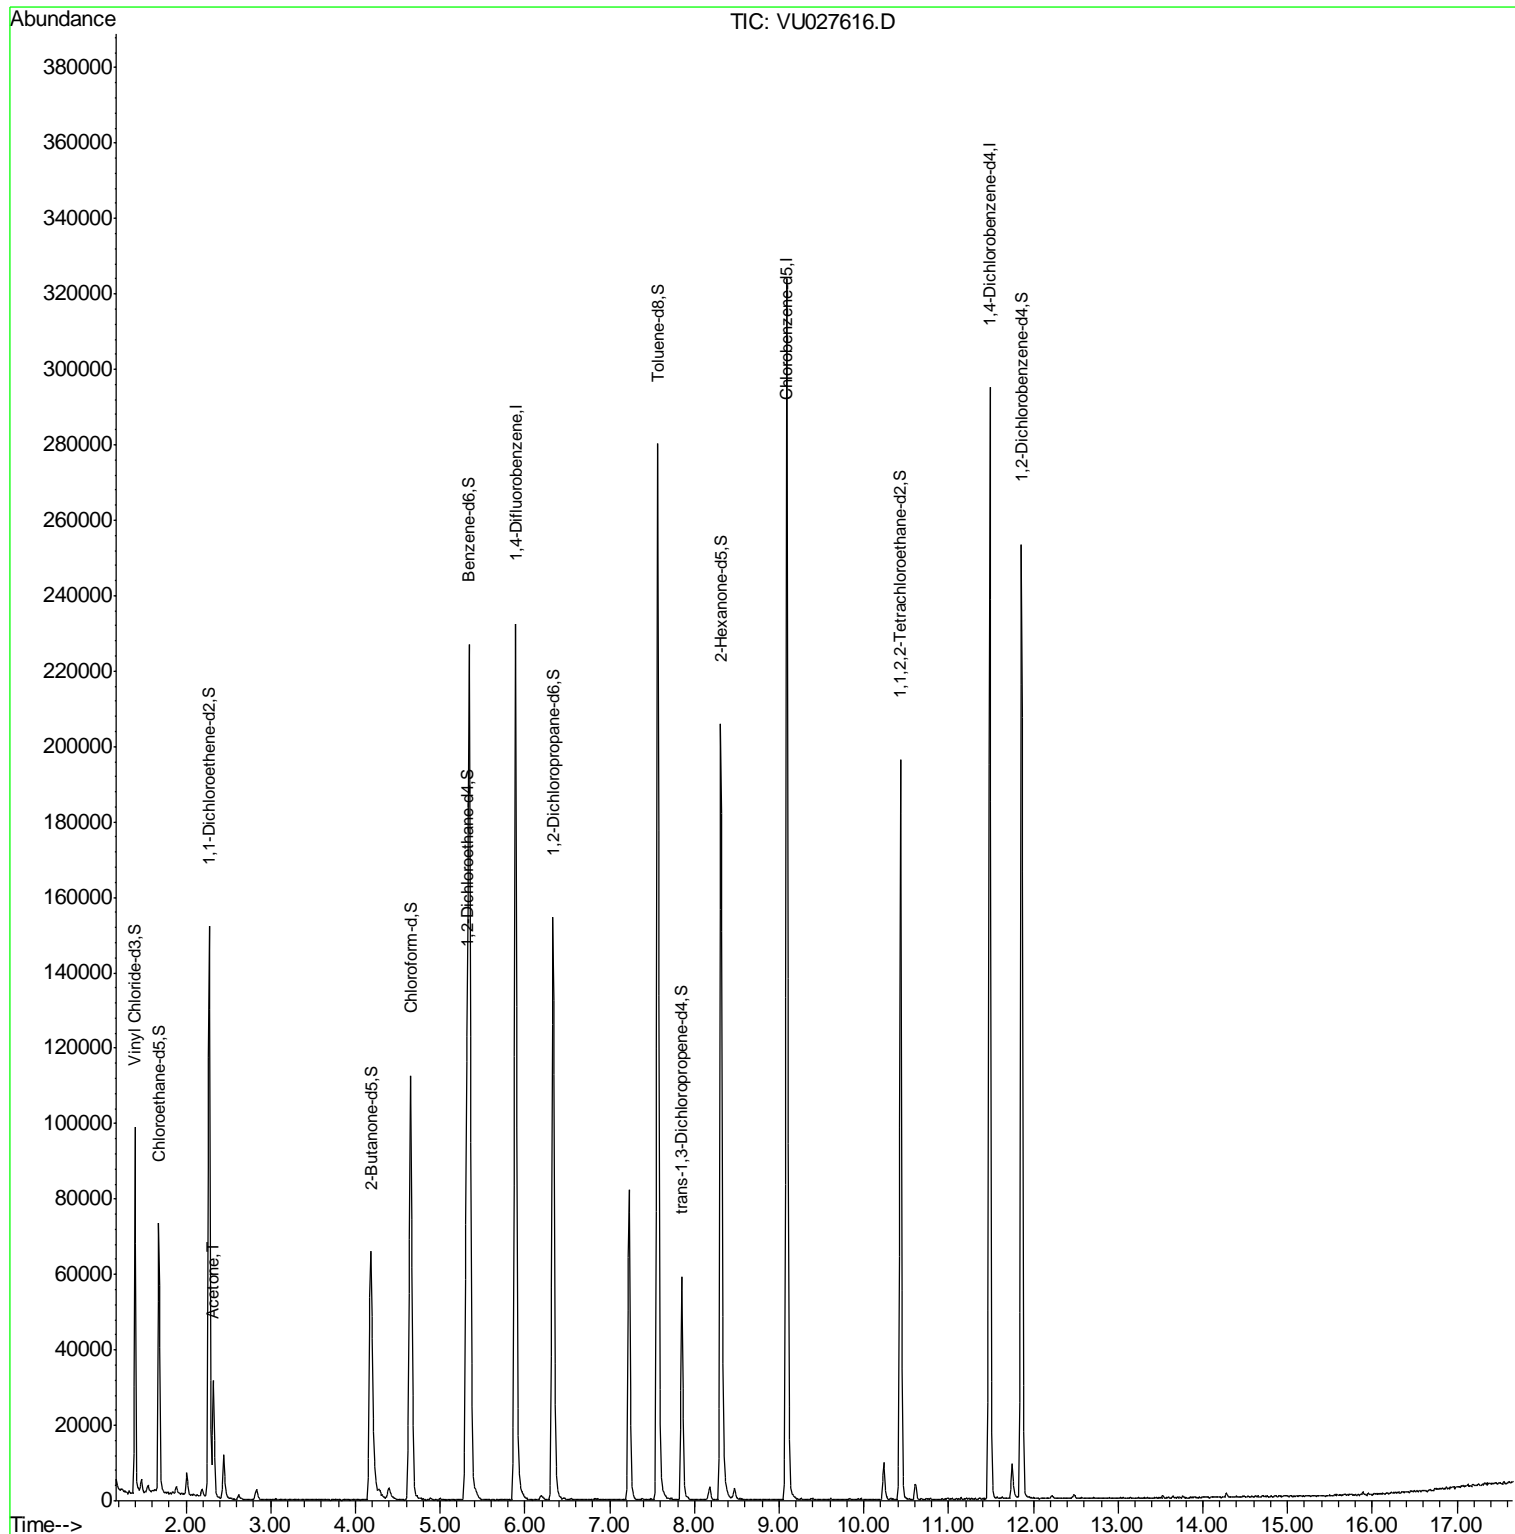

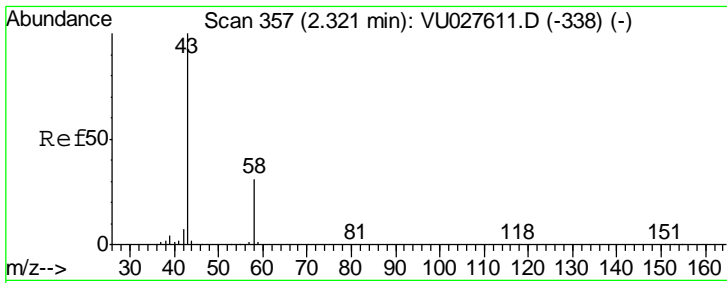

#13
 Acetone
 Concen: 32.315 ug/L
 RT: 2.32 min Scan# 358
 Delta R.T. 0.00 min
 Lab File: VU027616.D
 Acq: 12 Oct 2018 10:47

Instrument :
 MSVOA_U
 ClientSampled :
 C08X7

Tgt Ion: 43 Resp: 32530
 Ion Ratio Lower Upper
 43 100
 58 30.6 0.0 60.8

