

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
 Data File : VU027632.D
 Acq On : 12 Oct 2018 18:31
 Operator : MD/SY
 Sample : J5403-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0904

Quant Time: Oct 13 04:02:58 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 13 01:37:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	165868	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	155065	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	60975	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	52837	40.48	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	80.96%
7) Chloroethane-d5	1.68	69	43047	42.81	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.62%
11) 1,1-Dichloroethene-d2	2.27	63	73847	30.16	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	60.32%
21) 2-Butanone-d5	4.18	46	104497	99.16	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.16%
24) Chloroform-d	4.65	84	98933	47.39	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.78%
26) 1,2-Dichloroethane-d4	5.31	65	68524	46.84	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.68%
32) Benzene-d6	5.34	84	193258	43.49	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.98%
36) 1,2-Dichloropropane-d6	6.33	67	70698	46.44	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	92.88%
41) Toluene-d8	7.57	98	156611	39.43	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	78.86%#
43) trans-1,3-Dichloropropene-	7.85	79	29025	39.57	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.14%
47) 2-Hexanone-d5	8.31	63	71651	93.20	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.20%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	92359	46.40	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.80%
64) 1,2-Dichlorobenzene-d4	11.86	152	54850	45.98	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.96%


Target Compounds						Qvalue
13) Acetone	2.32	43	3315	3.84	ug/L	90
46) Tetrachloroethene	8.23	164	76402	83.89	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027632.D
Acq On : 12 Oct 2018 18:31
Operator : MD/SY
Sample : J5403-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0904

Quant Time: Oct 13 04:02:58 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 13 01:37:08 2018
Response via : Initial Calibration

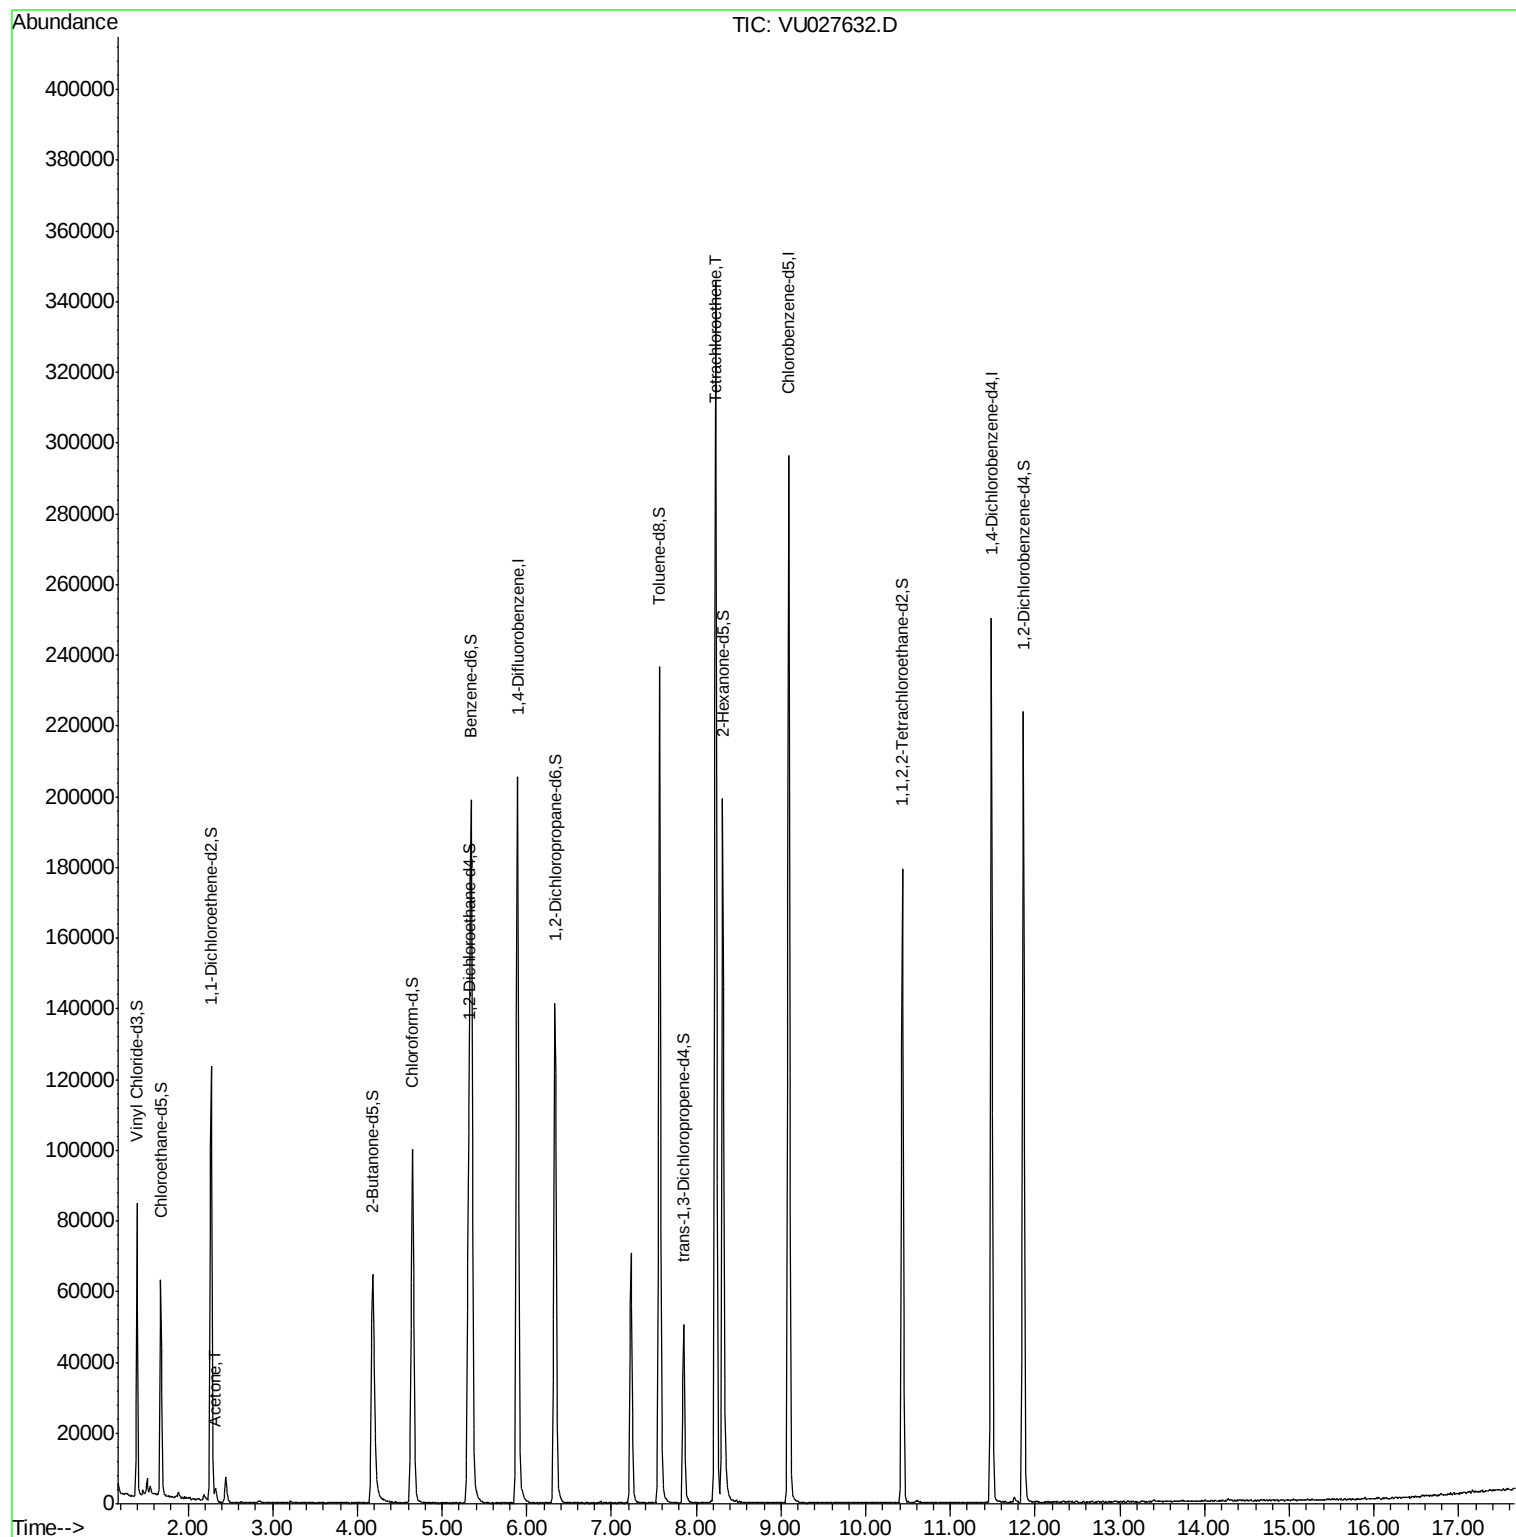

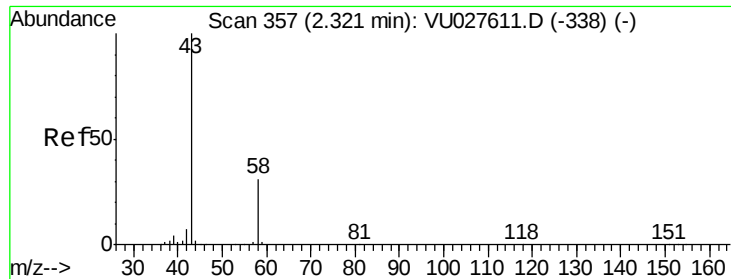

#13

Acetone

Concen: 3.84 ug/L

RT: 2.32 min Scan# 358

Delta R.T. 0.00 min

Lab File: VU027632.D

Acq: 12 Oct 2018 18:31

Instrument :

MSVOA_U

ClientSampleId :


C0904

Tgt Ion: 43 Resp: 3315

Ion Ratio Lower Upper




43 100

58 25.2 0.0 60.8

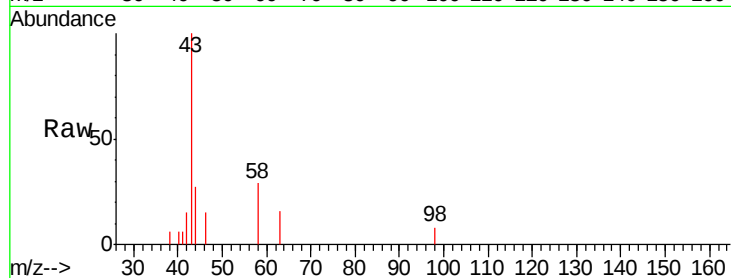

Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 58.00 (57.70 to 58.70): VU0

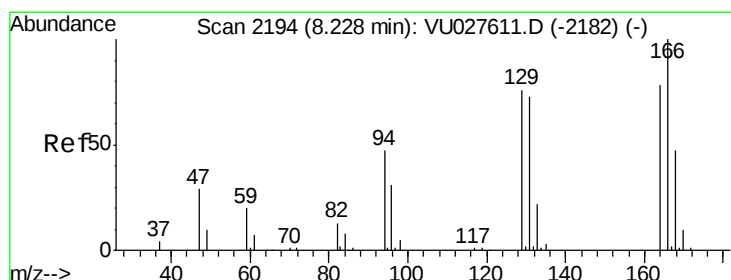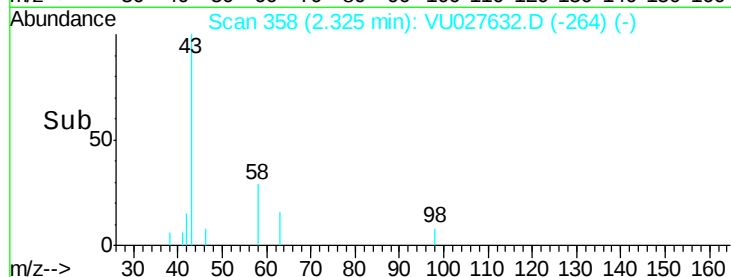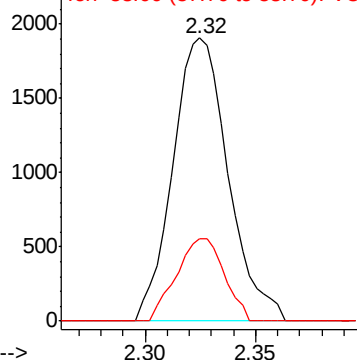

#46

Tetrachloroethene

Concen: 83.89 ug/L

RT: 8.23 min Scan# 2194

Delta R.T. 0.00 min

Lab File: VU027632.D

Acq: 12 Oct 2018 18:31

Tgt Ion: 164 Resp: 76402


Ion Ratio Lower Upper

164 100

129 94.7 67.0 124.4

131 90.1 65.1 120.9

166 127.9 90.4 167.8

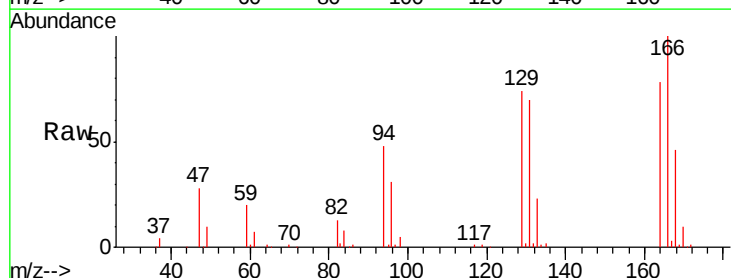

Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

