

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
 Data File : VU027613.D
 Acq On : 12 Oct 2018 09:38
 Operator : MD/SY
 Sample : J5380-03 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0T19

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.398	64	70	89	rVB	102969	105128	14.81%	2.027%
2	1.681	150	158	173	rVB	78553	99567	14.03%	1.920%
3	2.273	331	342	355	rBV	159851	244490	34.45%	4.715%
4	2.620	445	450	457	rBV2	344	420	0.06%	0.008%
5	2.668	462	465	468	rBV	160	114	0.02%	0.002%
6	2.704	469	476	481	rBV3	399	564	0.08%	0.011%
7	2.829	513	515	517	rBV	177	101	0.01%	0.002%
8	2.874	527	529	532	rBV	138	74	0.01%	0.001%
9	2.951	551	553	554	rBV	133	59	0.01%	0.001%
10	2.980	561	562	566	rVB	117	78	0.01%	0.002%
11	3.237	639	642	644	rBV	96	71	0.01%	0.001%
12	3.305	658	663	665	rBV	92	94	0.01%	0.002%
13	3.373	681	684	687	rBV	113	68	0.01%	0.001%
14	3.479	713	717	721	rBV	151	167	0.02%	0.003%
15	3.553	737	740	742	rVB2	194	110	0.02%	0.002%
16	3.678	777	779	782	rBV	101	66	0.01%	0.001%
17	3.752	800	802	805	rVB	134	54	0.01%	0.001%
18	3.819	821	823	827	rVB2	169	118	0.02%	0.002%
19	3.839	827	829	830	rBV	129	72	0.01%	0.001%
20	3.864	834	837	841	rVB	136	98	0.01%	0.002%
21	3.906	848	850	852	rVB	163	66	0.01%	0.001%
22	4.019	881	885	890	rBV	88	77	0.01%	0.001%
23	4.048	890	894	896	rVV	157	97	0.01%	0.002%
24	4.180	920	935	961	rBV	66629	175442	24.72%	3.383%
25	4.485	1028	1030	1032	rVB	195	89	0.01%	0.002%
26	4.565	1053	1055	1056	rBV	127	53	0.01%	0.001%
27	4.649	1065	1081	1110	rBV	114150	269020	37.91%	5.188%
28	4.823	1129	1135	1140	rBB2	155	148	0.02%	0.003%
29	4.858	1144	1146	1149	rVB	152	74	0.01%	0.001%
30	4.874	1149	1151	1152	rBV	132	54	0.01%	0.001%
31	4.890	1152	1156	1160	rVB	397	423	0.06%	0.008%
32	4.974	1177	1182	1185	rVB	64	56	0.01%	0.001%
33	4.993	1185	1188	1190	rBV	143	68	0.01%	0.001%
34	5.016	1193	1195	1198	rBV	92	62	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
 Data File : VU027613.D
 Acq On : 12 Oct 2018 09:38
 Operator : MD/SY
 Sample : J5380-03 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0T19

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

35	5.077	1209	1214	1219	rBV	147	149	0.02%	0.003%
36	5.202	1251	1253	1256	rBV	150	68	0.01%	0.001%
37	5.343	1273	1297	1325	rBV2	239709	709654	100.00%	13.685%
38	5.524	1350	1353	1355	rVB2	293	188	0.03%	0.004%
39	5.662	1393	1396	1399	rBV	174	87	0.01%	0.002%
40	5.790	1432	1436	1440	rVB2	193	142	0.02%	0.003%
41	5.829	1444	1448	1449	rBV	89	66	0.01%	0.001%
42	5.887	1452	1466	1494	rBV	211294	418454	58.97%	8.069%
43	6.093	1528	1530	1533	rBV2	158	123	0.02%	0.002%
44	6.138	1543	1544	1547	rVB	161	60	0.01%	0.001%
45	6.189	1550	1560	1572	rBV3	7175	13593	1.92%	0.262%
46	6.237	1572	1575	1579	rVB	105	80	0.01%	0.002%
47	6.282	1586	1589	1590	rBV	169	102	0.01%	0.002%
48	6.334	1590	1605	1628	rBV	162825	332844	46.90%	6.418%
49	6.462	1640	1645	1646	rBV2	426	368	0.05%	0.007%
50	6.659	1702	1706	1707	rBV	137	53	0.01%	0.001%
51	6.684	1710	1714	1715	rVB	145	65	0.01%	0.001%
52	6.707	1715	1721	1724	rBV	103	103	0.01%	0.002%
53	6.855	1763	1767	1769	rBV2	256	191	0.03%	0.004%
54	6.896	1777	1780	1783	rBV	527	448	0.06%	0.009%
55	7.083	1834	1838	1841	rBV	201	213	0.03%	0.004%
56	7.128	1850	1852	1853	rBV	139	59	0.01%	0.001%
57	7.186	1867	1870	1872	rBV	156	114	0.02%	0.002%
58	7.228	1872	1883	1908	rVV	88771	159065	22.41%	3.067%
59	7.398	1934	1936	1938	rBV	158	57	0.01%	0.001%
60	7.411	1938	1940	1943	rBV	246	114	0.02%	0.002%
61	7.456	1952	1954	1955	rBV	137	74	0.01%	0.001%
62	7.565	1973	1988	2021	rBV	300572	534810	75.36%	10.313%
63	7.742	2041	2043	2046	rBV2	295	138	0.02%	0.003%
64	7.774	2052	2053	2055	rVB2	252	89	0.01%	0.002%
65	7.851	2064	2077	2103	rBV	61532	106176	14.96%	2.047%
66	7.961	2109	2111	2112	rBV2	202	68	0.01%	0.001%
67	7.990	2117	2120	2123	rVB	230	152	0.02%	0.003%
68	8.019	2127	2129	2133	rVB	243	120	0.02%	0.002%
69	8.093	2149	2152	2154	rBV2	132	95	0.01%	0.002%
70	8.131	2160	2164	2166	rBV	219	198	0.03%	0.004%
71	8.160	2169	2173	2175	rBV	249	133	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
 Data File : VU027613.D
 Acq On : 12 Oct 2018 09:38
 Operator : MD/SY
 Sample : J5380-03 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0T19

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

72	8.176	2175	2178	2180	rBV	224	134	0.02%	0.003%
73	8.234	2188	2196	2205	rVB4	2995	4507	0.64%	0.087%
74	8.311	2208	2220	2251	rBV	209345	371676	52.37%	7.167%
75	8.575	2300	2302	2304	rBV	221	113	0.02%	0.002%
76	8.671	2330	2332	2333	rBV	173	55	0.01%	0.001%
77	8.732	2348	2351	2353	rBV2	180	124	0.02%	0.002%
78	8.781	2361	2366	2370	rBV2	237	304	0.04%	0.006%
79	8.922	2405	2410	2412	rBV2	200	142	0.02%	0.003%
80	9.093	2450	2463	2485	rBV	291397	491057	69.20%	9.469%
81	9.240	2506	2509	2510	rBV	216	98	0.01%	0.002%
82	9.376	2546	2551	2553	rBV2	323	303	0.04%	0.006%
83	9.404	2558	2560	2562	rBV2	162	86	0.01%	0.002%
84	9.520	2594	2596	2599	rVB	194	104	0.01%	0.002%
85	9.539	2599	2602	2604	rBV	230	153	0.02%	0.003%
86	9.745	2664	2666	2669	rBV	162	79	0.01%	0.002%
87	9.765	2670	2672	2676	rVV	152	56	0.01%	0.001%
88	9.826	2688	2691	2693	rBV	167	104	0.01%	0.002%
89	9.871	2702	2705	2708	rBV	136	101	0.01%	0.002%
90	9.929	2719	2723	2728	rBV2	231	189	0.03%	0.004%
91	10.064	2761	2765	2767	rBV2	202	172	0.02%	0.003%
92	10.160	2793	2795	2796	rBV2	133	60	0.01%	0.001%
93	10.308	2839	2841	2842	rBV	418	158	0.02%	0.003%
94	10.433	2868	2880	2900	rBV	198780	319481	45.02%	6.161%
95	10.777	2983	2987	2990	rBV2	238	218	0.03%	0.004%
96	11.076	3078	3080	3081	rBV2	176	61	0.01%	0.001%
97	11.424	3186	3188	3191	rVB	296	148	0.02%	0.003%
98	11.485	3195	3207	3223	rBV	259631	403622	56.88%	7.783%
99	11.861	3312	3324	3342	rBV	260354	416408	58.68%	8.030%
100	12.282	3452	3455	3461	rBV	276	298	0.04%	0.006%


Sum of corrected areas: 5185766

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027613.D
Acq On : 12 Oct 2018 09:38
Operator : MD/SY
Sample : J5380-03 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0T19

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

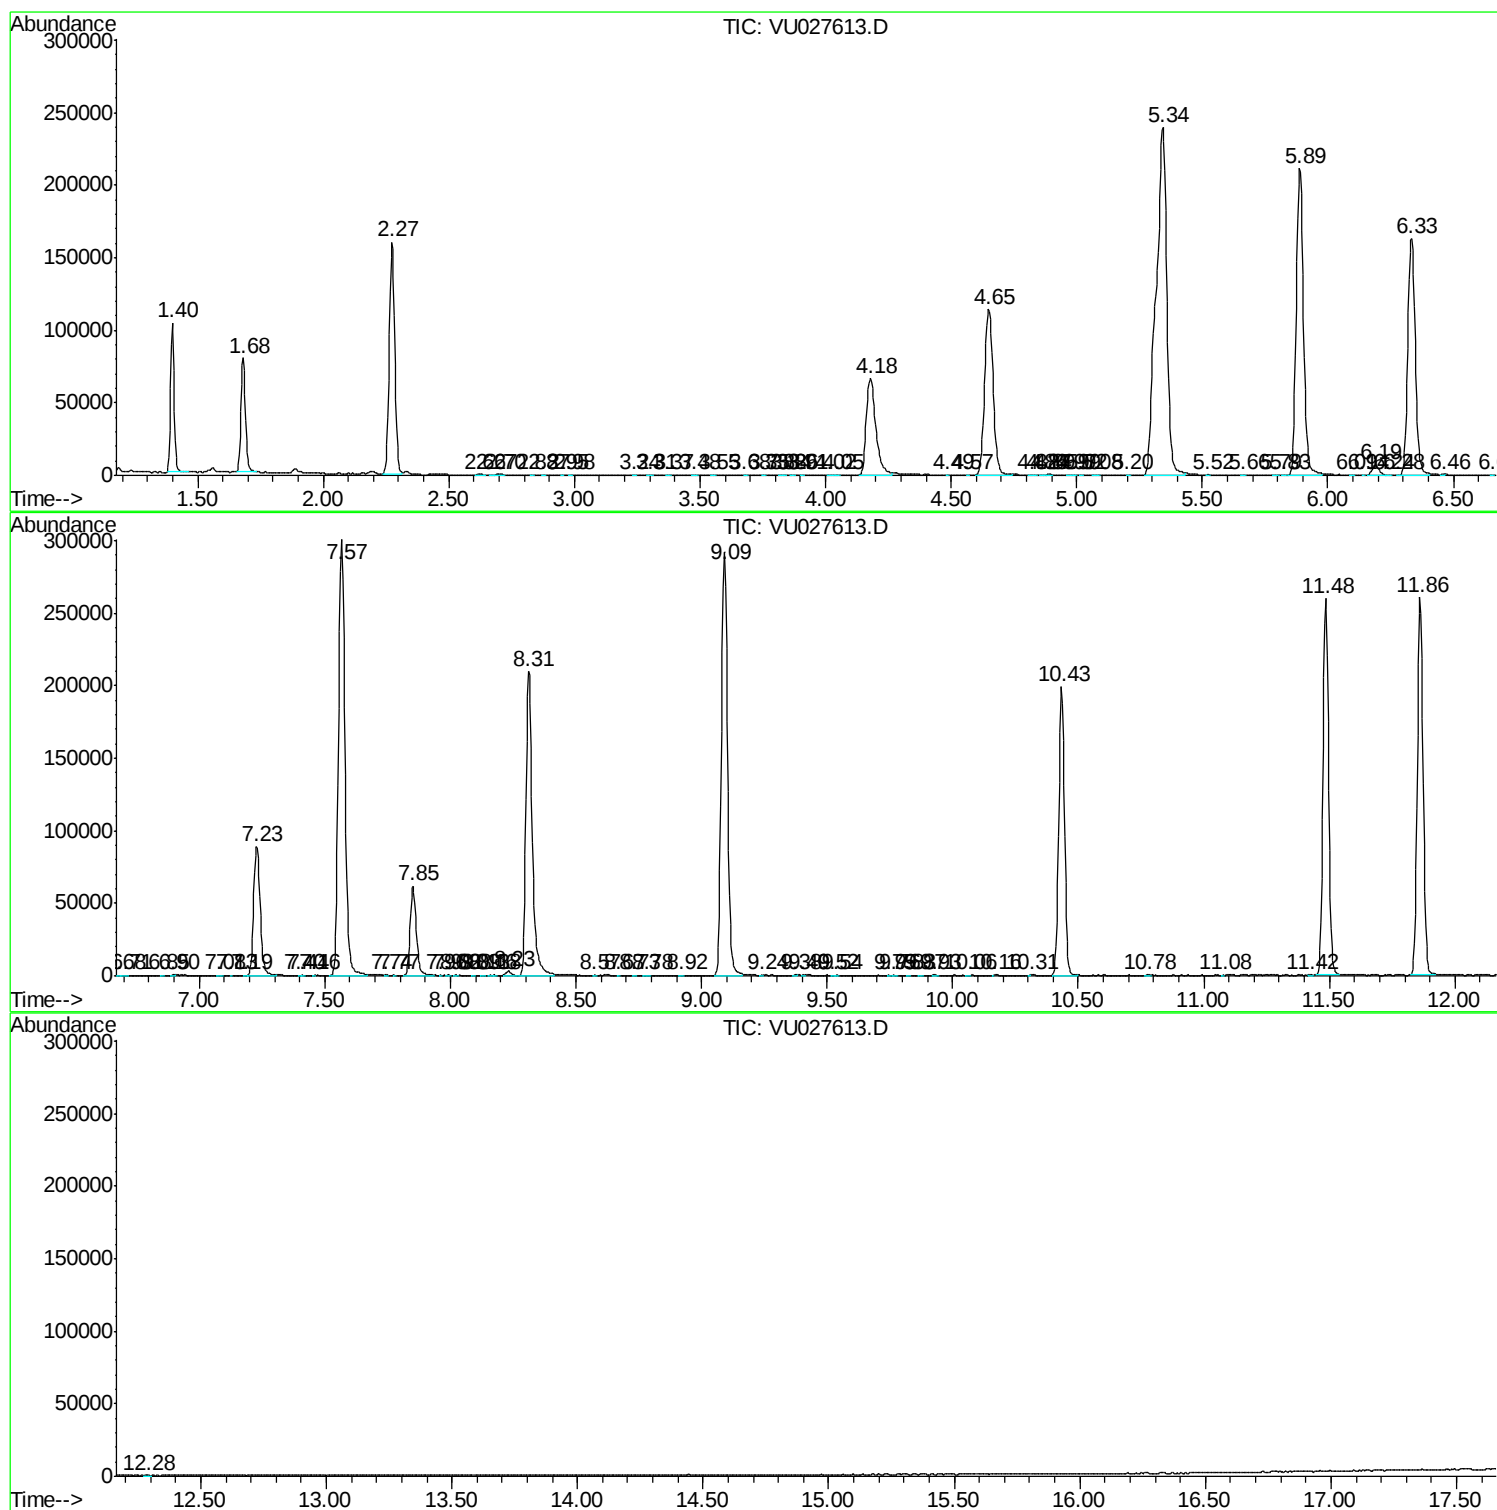

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027613.D
Acq On : 12 Oct 2018 09:38
Operator : MD/SY
Sample : J5380-03 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0T19

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027613.D
Acq On : 12 Oct 2018 09:38
Operator : MD/SY
Sample : J5380-03 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0T19

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc