

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
 Data File : VU027616.D
 Acq On : 12 Oct 2018 10:47
 Operator : MD/SY
 Sample : J5405-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08X7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.399	64	70	87	rBV	96645	99164	14.60%	1.887%
2	1.682	151	158	176	rVB	71371	90741	13.36%	1.727%
3	2.273	332	342	351	rBV	150707	227409	33.48%	4.327%
4	2.447	388	396	412	rVB	11353	19106	2.81%	0.364%
5	2.579	435	437	441	rVB	198	92	0.01%	0.002%
6	2.624	441	451	464	rVB3	1412	2415	0.36%	0.046%
7	2.717	477	480	482	rBV	213	143	0.02%	0.003%
8	2.836	505	517	525	rBV3	2755	5240	0.77%	0.100%
9	2.894	532	535	537	rBV	160	91	0.01%	0.002%
10	2.961	551	556	557	rBV	201	183	0.03%	0.003%
11	2.993	564	566	568	rVB	130	68	0.01%	0.001%
12	3.026	573	576	580	rBV	265	190	0.03%	0.004%
13	3.116	602	604	606	rVB	211	106	0.02%	0.002%
14	3.132	606	609	610	rBV	199	80	0.01%	0.002%
15	3.177	621	623	625	rBV	147	77	0.01%	0.001%
16	3.238	638	642	645	rBV2	187	125	0.02%	0.002%
17	3.260	645	649	652	rBV	145	105	0.02%	0.002%
18	3.418	695	698	703	rVB2	181	164	0.02%	0.003%
19	3.444	703	706	711	rVB2	161	105	0.02%	0.002%
20	3.501	721	724	727	rVB	164	145	0.02%	0.003%
21	3.540	733	736	739	rBV2	178	128	0.02%	0.002%
22	3.582	747	749	756	rVB	268	186	0.03%	0.004%
23	3.627	760	763	768	rBV2	189	191	0.03%	0.004%
24	3.669	768	776	779	rBV	197	244	0.04%	0.005%
25	3.720	788	792	794	rBV	217	165	0.02%	0.003%
26	3.736	795	797	800	rBV2	118	69	0.01%	0.001%
27	3.813	818	821	829	rVB2	245	310	0.05%	0.006%
28	3.871	837	839	842	rBV	125	90	0.01%	0.002%
29	3.894	844	846	850	rVB2	131	88	0.01%	0.002%
30	3.926	854	856	859	rVB2	175	95	0.01%	0.002%
31	4.022	883	886	890	rVB2	236	193	0.03%	0.004%
32	4.045	891	893	896	rVB2	225	123	0.02%	0.002%
33	4.074	896	902	907	rBV	228	230	0.03%	0.004%
34	4.103	909	911	915	rBV2	113	93	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
 Data File : VU027616.D
 Acq On : 12 Oct 2018 10:47
 Operator : MD/SY
 Sample : J5405-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08X7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

35	4.183	922	936	961	rBV	65877	183160	26.97%	3.485%
36	4.524	1038	1042	1047	rBV3	238	247	0.04%	0.005%
37	4.653	1065	1082	1103	rBV	112597	263763	38.84%	5.019%
38	4.884	1148	1154	1160	rBV2	508	697	0.10%	0.013%
39	4.942	1166	1172	1176	rBV	96	95	0.01%	0.002%
40	4.961	1176	1178	1182	rVB	168	72	0.01%	0.001%
41	4.990	1182	1187	1188	rBV	406	330	0.05%	0.006%
42	5.035	1199	1201	1203	rBV	158	86	0.01%	0.002%
43	5.051	1203	1206	1210	rVB	161	107	0.02%	0.002%
44	5.212	1253	1256	1261	rVB	125	87	0.01%	0.002%
45	5.238	1261	1264	1269	rBV	95	91	0.01%	0.002%
46	5.344	1273	1297	1338	rBV2	227001	679171	100.00%	12.924%
47	5.527	1353	1354	1358	rVB2	181	93	0.01%	0.002%
48	5.546	1358	1360	1364	rVB	133	110	0.02%	0.002%
49	5.678	1398	1401	1404	rVB2	215	144	0.02%	0.003%
50	5.890	1449	1467	1501	rBV	232452	471123	69.37%	8.965%
51	6.122	1537	1539	1546	rBV	183	166	0.02%	0.003%
52	6.180	1549	1557	1558	rBV3	909	741	0.11%	0.014%
53	6.334	1590	1605	1629	rBV	154371	316846	46.65%	6.029%
54	6.546	1667	1671	1673	rVV2	246	173	0.03%	0.003%
55	6.575	1678	1680	1683	rBV	230	102	0.02%	0.002%
56	6.820	1754	1756	1759	rBV3	223	127	0.02%	0.002%
57	6.855	1764	1767	1768	rBV	218	142	0.02%	0.003%
58	6.916	1783	1786	1788	rBV	185	113	0.02%	0.002%
59	6.990	1805	1809	1812	rBV	88	69	0.01%	0.001%
60	7.080	1835	1837	1840	rBV	135	67	0.01%	0.001%
61	7.112	1845	1847	1849	rVB	170	73	0.01%	0.001%
62	7.231	1872	1884	1901	rBV	82367	147889	21.77%	2.814%
63	7.350	1918	1921	1925	rVB2	190	129	0.02%	0.002%
64	7.389	1931	1933	1934	rBV2	273	79	0.01%	0.002%
65	7.472	1954	1959	1962	rBV	321	341	0.05%	0.006%
66	7.517	1971	1973	1976	rBV2	151	98	0.01%	0.002%
67	7.569	1976	1989	2008	rBV	280080	500845	73.74%	9.531%
68	7.852	2066	2077	2097	rVV	59257	101032	14.88%	1.923%
69	7.971	2111	2114	2116	rBV	255	134	0.02%	0.003%
70	8.022	2126	2130	2132	rBV2	162	102	0.02%	0.002%
71	8.074	2143	2146	2150	rBV	159	114	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
 Data File : VU027616.D
 Acq On : 12 Oct 2018 10:47
 Operator : MD/SY
 Sample : J5405-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08X7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

72	8.115	2157	2159	2164	rVV	165	108	0.02%	0.002%
73	8.180	2168	2179	2194	rVV2	3475	6372	0.94%	0.121%
74	8.267	2203	2206	2208	rBV	174	132	0.02%	0.003%
75	8.312	2208	2220	2248	rBV	205785	362451	53.37%	6.897%
76	8.553	2292	2295	2296	rBV	251	136	0.02%	0.003%
77	8.585	2303	2305	2308	rBV2	158	100	0.01%	0.002%
78	8.656	2325	2327	2332	rVB2	192	119	0.02%	0.002%
79	8.678	2332	2334	2335	rBV2	170	77	0.01%	0.001%
80	8.723	2346	2348	2350	rBV	118	65	0.01%	0.001%
81	8.765	2359	2361	2364	rBV	161	111	0.02%	0.002%
82	8.916	2404	2408	2412	rBV2	182	143	0.02%	0.003%
83	8.939	2413	2415	2419	rBV2	142	118	0.02%	0.002%
84	8.971	2424	2425	2430	rVV	205	101	0.01%	0.002%
85	9.006	2433	2436	2439	rVB	216	122	0.02%	0.002%
86	9.090	2450	2462	2483	rBV	323861	548601	80.78%	10.440%
87	9.244	2503	2510	2511	rBV2	223	282	0.04%	0.005%
88	9.376	2548	2551	2552	rBV2	262	139	0.02%	0.003%
89	9.598	2617	2620	2621	rBV	163	91	0.01%	0.002%
90	9.836	2691	2694	2697	rVB	213	137	0.02%	0.003%
91	9.916	2715	2719	2721	rBV	268	196	0.03%	0.004%
92	10.234	2809	2818	2833	rBB	9934	17103	2.52%	0.325%
93	10.292	2833	2836	2837	rBV	159	77	0.01%	0.001%
94	10.434	2867	2880	2899	rBV	196185	310699	45.75%	5.912%
95	10.607	2926	2934	2945	rBV3	3993	6438	0.95%	0.123%
96	10.958	3040	3043	3045	rBV	205	102	0.02%	0.002%
97	11.485	3195	3207	3224	rBV	294766	459537	67.66%	8.745%
98	11.749	3281	3289	3306	rBV2	9084	15404	2.27%	0.293%
99	11.861	3312	3324	3339	rBV	252724	408882	60.20%	7.781%
100	12.572	3542	3545	3551	rVB3	510	465	0.07%	0.009%


Sum of corrected areas: 5255020

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027616.D
Acq On : 12 Oct 2018 10:47
Operator : MD/SY
Sample : J5405-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
C08X7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

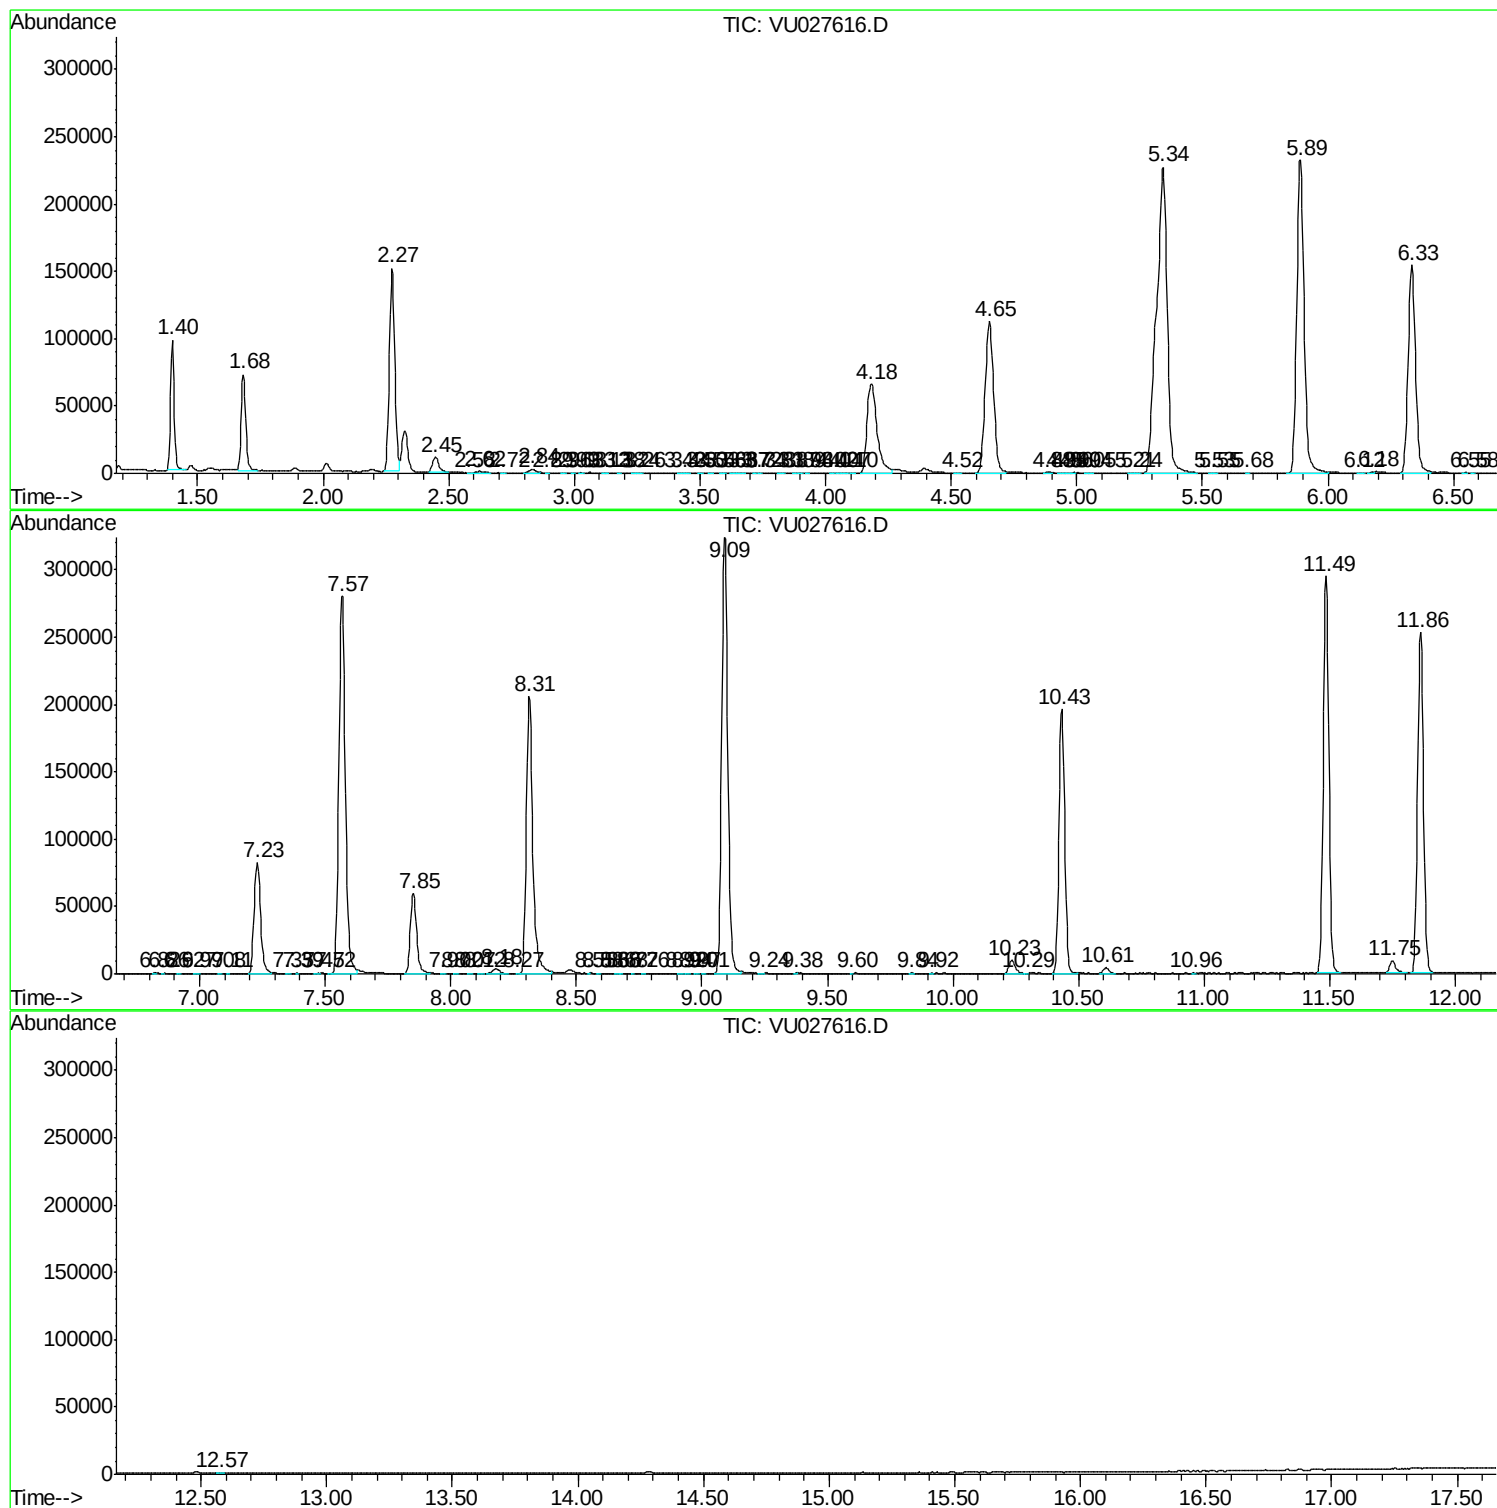

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027616.D
Acq On : 12 Oct 2018 10:47
Operator : MD/SY
Sample : J5405-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08X7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027616.D
Acq On : 12 Oct 2018 10:47
Operator : MD/SY
Sample : J5405-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08X7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc