

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
 Data File : VU027635.D
 Acq On : 12 Oct 2018 20:04
 Operator : MD/SY
 Sample : VU1012WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK57

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.398	64	70	81	rBV	93789	96090	14.68%	1.973%
2	1.681	151	158	176	rVB	68479	87008	13.29%	1.786%
3	2.273	332	342	357	rBV	142331	218516	33.39%	4.486%
4	2.553	427	429	434	rVB	193	104	0.02%	0.002%
5	2.694	470	473	474	rBV	329	189	0.03%	0.004%
6	2.839	515	518	520	rBV	155	84	0.01%	0.002%
7	2.987	562	564	565	rBV	130	54	0.01%	0.001%
8	3.228	634	639	643	rBV2	243	258	0.04%	0.005%
9	3.305	660	663	664	rBV2	156	76	0.01%	0.002%
10	3.479	715	717	718	rBV2	155	47	0.01%	0.001%
11	3.501	722	724	729	rVB	168	91	0.01%	0.002%
12	3.585	749	750	755	rVB	221	96	0.01%	0.002%
13	3.614	755	759	761	rBV	128	108	0.02%	0.002%
14	3.630	761	764	766	rVV	185	150	0.02%	0.003%
15	3.659	770	773	776	rBV	102	62	0.01%	0.001%
16	3.723	791	793	797	rBV	81	46	0.01%	0.001%
17	3.762	802	805	808	rBV	75	63	0.01%	0.001%
18	3.935	855	859	862	rVB	181	97	0.01%	0.002%
19	3.958	862	866	870	rBV	97	97	0.01%	0.002%
20	4.012	879	883	884	rBV	96	66	0.01%	0.001%
21	4.048	891	894	899	rVB	86	72	0.01%	0.001%
22	4.074	899	902	905	rBV	103	86	0.01%	0.002%
23	4.180	922	935	969	rBV	62242	165615	25.31%	3.400%
24	4.514	1037	1039	1041	rBV	146	85	0.01%	0.002%
25	4.549	1049	1050	1054	rVB	126	88	0.01%	0.002%
26	4.572	1055	1057	1059	rBV	126	40	0.01%	0.001%
27	4.652	1066	1082	1108	rBV	106044	251917	38.49%	5.172%
28	4.842	1135	1141	1143	rBV2	177	131	0.02%	0.003%
29	4.858	1143	1146	1149	rBV	217	189	0.03%	0.004%
30	4.881	1149	1153	1154	rBV2	327	220	0.03%	0.005%
31	4.938	1168	1171	1173	rBV	149	112	0.02%	0.002%
32	4.958	1175	1177	1181	rVV	158	83	0.01%	0.002%
33	4.977	1181	1183	1188	rVB2	166	148	0.02%	0.003%
34	5.019	1193	1196	1197	rBV	178	89	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
 Data File : VU027635.D
 Acq On : 12 Oct 2018 20:04
 Operator : MD/SY
 Sample : VU1012WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK57

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

35	5.099	1218	1221	1226	rVB2	162	154	0.02%	0.003%
36	5.135	1226	1232	1234	rBV2	175	192	0.03%	0.004%
37	5.196	1249	1251	1252	rBV2	99	41	0.01%	0.001%
38	5.208	1252	1255	1258	rBV2	165	115	0.02%	0.002%
39	5.221	1258	1259	1265	rVB2	158	62	0.01%	0.001%
40	5.254	1265	1269	1271	rBV	188	112	0.02%	0.002%
41	5.344	1272	1297	1330	rBV2	220327	654445	100.00%	13.436%
42	5.553	1359	1362	1365	rVB3	238	141	0.02%	0.003%
43	5.665	1392	1397	1399	rBV	215	114	0.02%	0.002%
44	5.678	1399	1401	1404	rVV	143	52	0.01%	0.001%
45	5.890	1453	1467	1499	rBV	218517	431759	65.97%	8.864%
46	6.080	1524	1526	1529	rVB2	173	108	0.02%	0.002%
47	6.128	1539	1541	1542	rBV2	140	58	0.01%	0.001%
48	6.180	1552	1557	1563	rBV2	698	818	0.12%	0.017%
49	6.334	1591	1605	1638	rBV	152735	306946	46.90%	6.302%
50	6.498	1654	1656	1659	rVB	233	90	0.01%	0.002%
51	6.517	1659	1662	1663	rBV	85	47	0.01%	0.001%
52	6.572	1676	1679	1683	rVB2	193	120	0.02%	0.002%
53	6.713	1717	1723	1724	rBV	102	98	0.01%	0.002%
54	6.861	1765	1769	1770	rBV	215	174	0.03%	0.004%
55	6.922	1786	1788	1789	rBV	143	61	0.01%	0.001%
56	6.958	1796	1799	1804	rBV	84	78	0.01%	0.002%
57	7.077	1833	1836	1838	rBV	72	49	0.01%	0.001%
58	7.151	1856	1859	1863	rBV	120	91	0.01%	0.002%
59	7.179	1866	1868	1871	rVB	174	57	0.01%	0.001%
60	7.231	1871	1884	1909	rBV	75527	136449	20.85%	2.801%
61	7.337	1915	1917	1919	rBV	121	36	0.01%	0.001%
62	7.353	1921	1922	1923	rBV	128	38	0.01%	0.001%
63	7.495	1963	1966	1968	rVB	73	33	0.01%	0.001%
64	7.569	1975	1989	2008	rBV	267159	473894	72.41%	9.729%
65	7.742	2039	2043	2047	rBV2	125	108	0.02%	0.002%
66	7.778	2052	2054	2055	rBV2	170	77	0.01%	0.002%
67	7.851	2066	2077	2099	rBV	53430	92285	14.10%	1.895%
68	8.147	2167	2169	2171	rVB2	151	80	0.01%	0.002%
69	8.163	2171	2174	2176	rBV	334	256	0.04%	0.005%
70	8.212	2187	2189	2191	rBV	69	36	0.01%	0.001%
71	8.237	2191	2197	2202	rBV5	1083	1386	0.21%	0.028%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027635.D
Acq On : 12 Oct 2018 20:04
Operator : MD/SY
Sample : VU1012WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK57

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Title : VOC Analysis

72	8.314	2209	2221	2250	rBV	194483	348287	53.22%	7.150%
73	8.581	2302	2304	2305	rBV	174	69	0.01%	0.001%
74	8.614	2311	2314	2315	rBV2	439	222	0.03%	0.005%
75	8.713	2341	2345	2348	rBV	109	111	0.02%	0.002%
76	8.745	2352	2355	2359	rVB	162	106	0.02%	0.002%
77	8.822	2376	2379	2383	rBV	188	119	0.02%	0.002%
78	8.896	2400	2402	2404	rBV	176	89	0.01%	0.002%
79	9.093	2450	2463	2485	rBV	305688	512244	78.27%	10.516%
80	9.376	2548	2551	2554	rBV2	264	193	0.03%	0.004%
81	9.639	2631	2633	2636	rVB	192	63	0.01%	0.001%
82	9.732	2658	2662	2666	rBV2	290	269	0.04%	0.006%
83	9.806	2682	2685	2686	rBV	229	132	0.02%	0.003%
84	9.842	2694	2696	2698	rBV	165	95	0.01%	0.002%
85	9.867	2701	2704	2709	rVB	172	124	0.02%	0.003%
86	10.003	2742	2746	2749	rBV2	167	122	0.02%	0.003%
87	10.131	2783	2786	2787	rBV	151	69	0.01%	0.001%
88	10.266	2825	2828	2831	rBV2	204	165	0.03%	0.003%
89	10.433	2868	2880	2899	rBV	190416	298513	45.61%	6.128%
90	10.565	2918	2921	2924	rBV2	190	135	0.02%	0.003%
91	10.665	2949	2952	2956	rVB2	223	156	0.02%	0.003%
92	10.684	2956	2958	2962	rBV	168	66	0.01%	0.001%
93	10.790	2989	2991	2999	rBV	224	265	0.04%	0.005%
94	10.900	3024	3025	3026	rBV	123	30	0.00%	0.001%
95	11.170	3107	3109	3110	rBV	157	46	0.01%	0.001%
96	11.485	3195	3207	3232	rBV	259375	408496	62.42%	8.386%
97	11.629	3250	3252	3253	rBV	201	89	0.01%	0.002%
98	11.646	3255	3257	3260	rVB2	267	130	0.02%	0.003%
99	11.861	3312	3324	3341	rBV	235749	377551	57.69%	7.751%
100	13.096	3706	3708	3710	rBV	265	171	0.03%	0.004%


Sum of corrected areas: 4870964

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027635.D
Acq On : 12 Oct 2018 20:04
Operator : MD/SY
Sample : VU1012WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK57

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

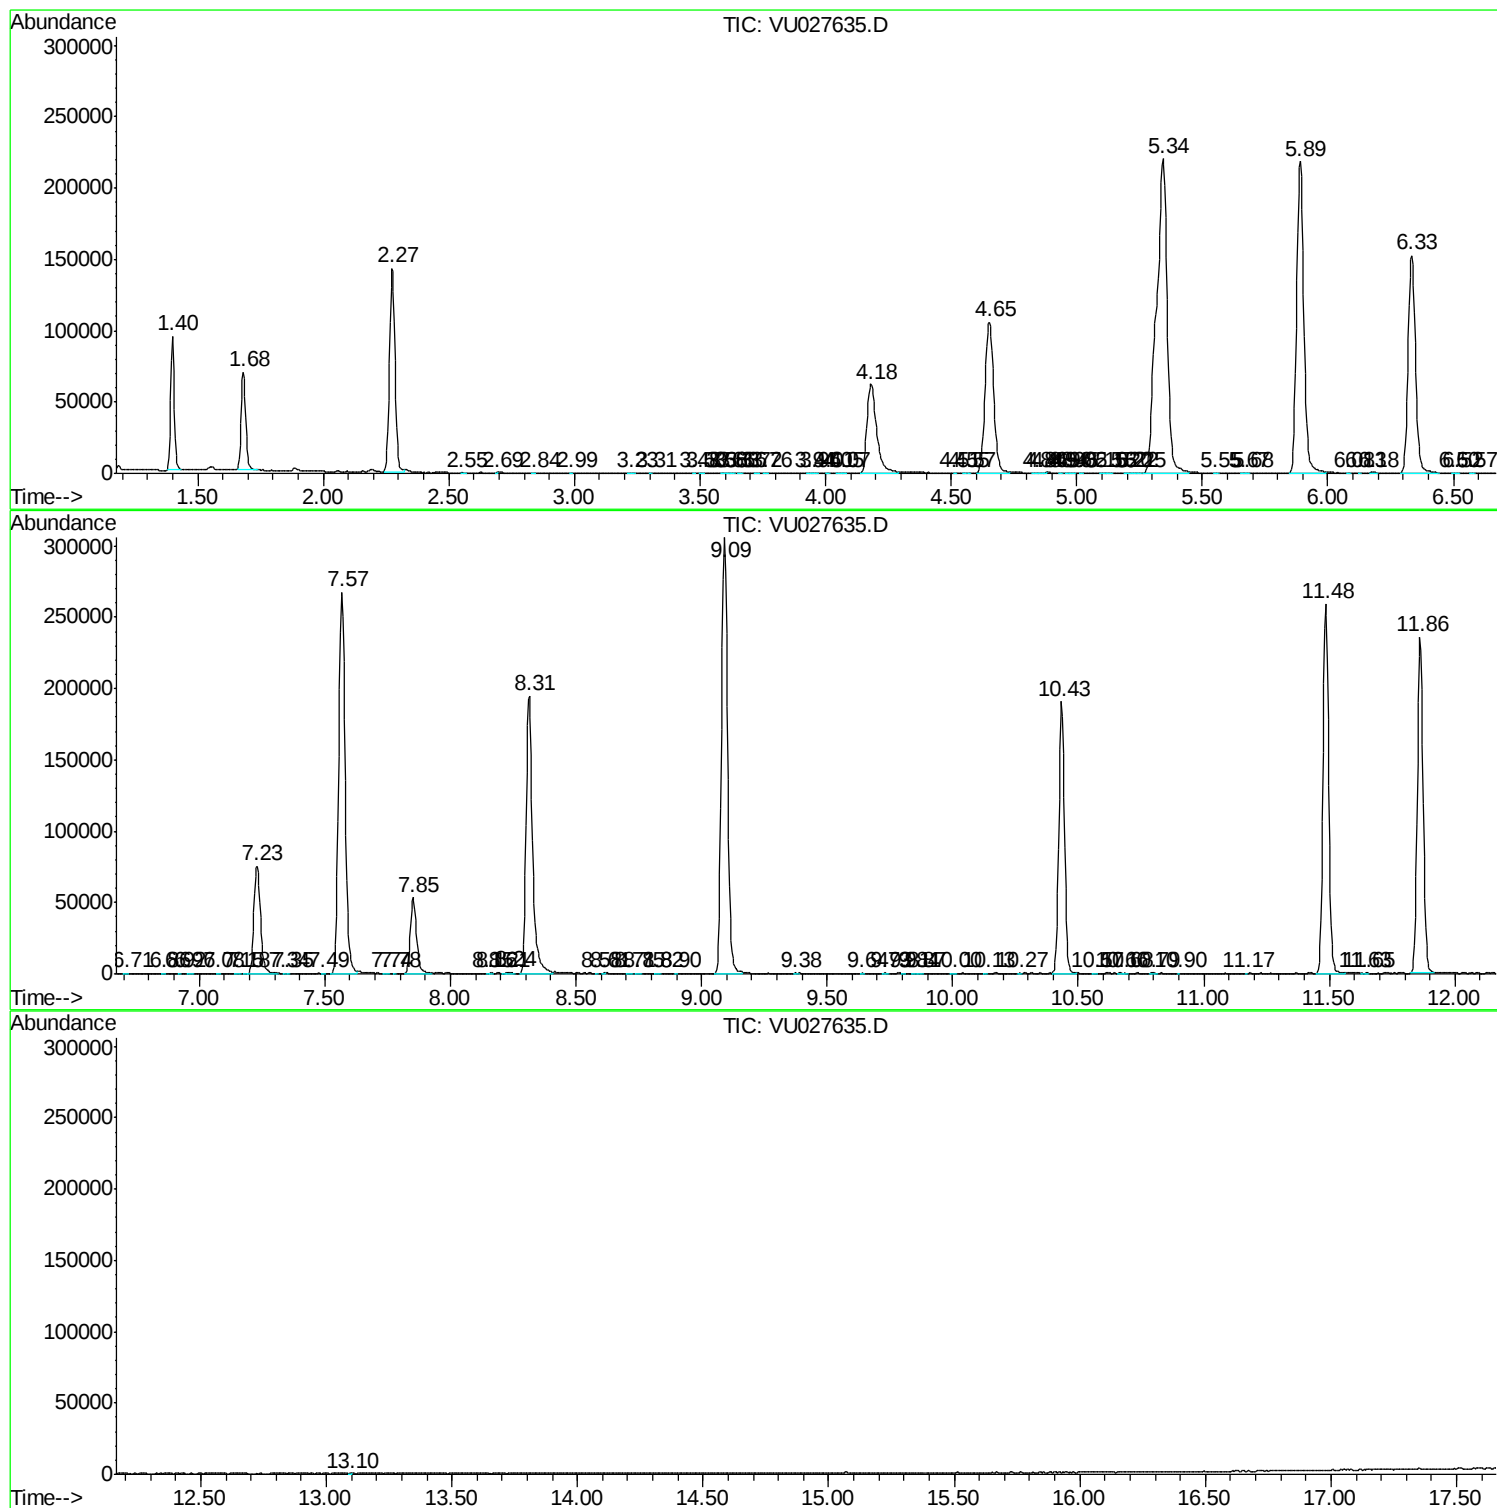

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027635.D
Acq On : 12 Oct 2018 20:04
Operator : MD/SY
Sample : VU1012WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK57

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027635.D
Acq On : 12 Oct 2018 20:04
Operator : MD/SY
Sample : VU1012WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK57

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc