

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
 Data File : VU027640.D
 Acq On : 12 Oct 2018 22:00
 Operator : MD/SY
 Sample : J5405-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08Y0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.398	64	70	82	rBV	81204	83078	13.68%	1.821%
2	1.681	151	158	182	rVB	63019	83567	13.76%	1.831%
3	2.276	332	343	354	rBV	123685	189539	31.21%	4.154%
4	2.411	382	385	386	rBV	196	105	0.02%	0.002%
5	2.443	386	395	410	rVV	7945	13886	2.29%	0.304%
6	2.578	434	437	442	rVB	214	138	0.02%	0.003%
7	2.842	512	519	525	rVB2	644	882	0.15%	0.019%
8	3.032	576	578	579	rBV2	128	54	0.01%	0.001%
9	3.144	610	613	616	rBV	144	99	0.02%	0.002%
10	3.315	663	666	668	rBV	117	75	0.01%	0.002%
11	3.479	716	717	720	rVB	167	42	0.01%	0.001%
12	3.623	760	762	766	rVB	150	70	0.01%	0.002%
13	3.646	766	769	771	rBV	115	77	0.01%	0.002%
14	3.775	806	809	812	rBV2	225	154	0.03%	0.003%
15	3.810	817	820	824	rVB	70	54	0.01%	0.001%
16	3.832	824	827	828	rBV	207	96	0.02%	0.002%
17	3.906	846	850	851	rBV	108	75	0.01%	0.002%
18	4.019	879	885	889	rBV	127	134	0.02%	0.003%
19	4.054	893	896	899	rBV	78	52	0.01%	0.001%
20	4.180	921	935	960	rBV	65521	176847	29.12%	3.876%
21	4.453	1017	1020	1022	rBV2	157	128	0.02%	0.003%
22	4.520	1038	1041	1045	rVB	153	97	0.02%	0.002%
23	4.652	1062	1082	1107	rBV	100788	237097	39.04%	5.196%
24	4.800	1125	1128	1130	rBV	69	41	0.01%	0.001%
25	4.839	1137	1140	1144	rBV	102	94	0.02%	0.002%
26	4.855	1144	1145	1147	rVB	110	42	0.01%	0.001%
27	4.890	1148	1156	1157	rBV	249	214	0.04%	0.005%
28	4.964	1171	1179	1181	rBV	83	105	0.02%	0.002%
29	5.086	1212	1217	1219	rBV	58	51	0.01%	0.001%
30	5.144	1231	1235	1238	rBV	72	57	0.01%	0.001%
31	5.164	1238	1241	1246	rBV	69	80	0.01%	0.002%
32	5.225	1253	1260	1265	rBV	127	165	0.03%	0.004%
33	5.250	1266	1268	1272	rVB	149	72	0.01%	0.002%
34	5.344	1273	1297	1326	rBV2	201780	607291	100.00%	13.310%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
 Data File : VU027640.D
 Acq On : 12 Oct 2018 22:00
 Operator : MD/SY
 Sample : J5405-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08Y0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

35	5.533	1355	1356	1362	rBV	234	150	0.02%	0.003%
36	5.572	1367	1368	1371	rVB	162	61	0.01%	0.001%
37	5.594	1371	1375	1379	rBV	86	99	0.02%	0.002%
38	5.781	1431	1433	1434	rBV	120	49	0.01%	0.001%
39	5.890	1453	1467	1495	rBV	201772	401185	66.06%	8.792%
40	6.157	1545	1550	1553	rBV	88	86	0.01%	0.002%
41	6.176	1553	1556	1562	rVB2	494	473	0.08%	0.010%
42	6.257	1577	1581	1584	rBV	113	84	0.01%	0.002%
43	6.334	1591	1605	1637	rBV	144422	291276	47.96%	6.384%
44	6.463	1642	1645	1650	rVB2	395	312	0.05%	0.007%
45	6.681	1711	1713	1715	rVV	152	67	0.01%	0.001%
46	6.694	1715	1717	1720	rVB	94	47	0.01%	0.001%
47	6.745	1730	1733	1735	rBV2	173	107	0.02%	0.002%
48	6.861	1764	1769	1779	rVB4	455	662	0.11%	0.015%
49	6.903	1779	1782	1787	rBV	83	87	0.01%	0.002%
50	6.987	1805	1808	1810	rBV	59	41	0.01%	0.001%
51	7.028	1818	1821	1824	rBV	63	46	0.01%	0.001%
52	7.109	1843	1846	1854	rVV	165	108	0.02%	0.002%
53	7.160	1858	1862	1866	rBV	64	69	0.01%	0.002%
54	7.231	1871	1884	1905	rBV	70247	126742	20.87%	2.778%
55	7.344	1916	1919	1921	rBV	66	44	0.01%	0.001%
56	7.360	1922	1924	1926	rVV	141	47	0.01%	0.001%
57	7.385	1930	1932	1936	rVB	194	146	0.02%	0.003%
58	7.408	1936	1939	1941	rBV	82	52	0.01%	0.001%
59	7.569	1975	1989	2022	rBV	236571	425251	70.02%	9.320%
60	7.768	2049	2051	2056	rVB	245	127	0.02%	0.003%
61	7.790	2056	2058	2063	rBV	182	123	0.02%	0.003%
62	7.852	2066	2077	2100	rBV	50470	85225	14.03%	1.868%
63	7.967	2110	2113	2115	rVB	286	155	0.03%	0.003%
64	7.996	2115	2122	2124	rBV2	234	211	0.03%	0.005%
65	8.041	2134	2136	2138	rBV	152	78	0.01%	0.002%
66	8.180	2171	2179	2189	rBV	1286	1801	0.30%	0.039%
67	8.225	2192	2193	2195	rVV	116	46	0.01%	0.001%
68	8.311	2209	2220	2251	rBV	192704	349395	57.53%	7.657%
69	8.630	2316	2319	2322	rBV	222	192	0.03%	0.004%
70	8.742	2349	2354	2356	rBV2	195	158	0.03%	0.003%
71	8.774	2361	2364	2366	rBV	192	96	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
 Data File : VU027640.D
 Acq On : 12 Oct 2018 22:00
 Operator : MD/SY
 Sample : J5405-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08Y0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

72	8.848	2384	2387	2388	rBV	136	84	0.01%	0.002%
73	8.858	2388	2390	2394	rVV2	171	142	0.02%	0.003%
74	8.967	2422	2424	2425	rBV	100	38	0.01%	0.001%
75	9.089	2450	2462	2489	rBV	279709	474627	78.15%	10.402%
76	9.237	2505	2508	2509	rBV2	231	121	0.02%	0.003%
77	9.282	2518	2522	2531	rBV	190	214	0.04%	0.005%
78	9.321	2531	2534	2537	rBV2	263	170	0.03%	0.004%
79	9.340	2537	2540	2546	rVB	144	172	0.03%	0.004%
80	9.437	2567	2570	2573	rBV2	158	105	0.02%	0.002%
81	9.581	2613	2615	2618	rBV	145	119	0.02%	0.003%
82	9.736	2660	2663	2665	rBV	183	97	0.02%	0.002%
83	9.826	2687	2691	2693	rBV	246	179	0.03%	0.004%
84	9.893	2710	2712	2714	rBV2	145	95	0.02%	0.002%
85	9.925	2720	2722	2726	rVB	200	107	0.02%	0.002%
86	10.003	2744	2746	2747	rBV	179	81	0.01%	0.002%
87	10.083	2769	2771	2775	rVB	172	68	0.01%	0.001%
88	10.228	2813	2816	2819	rBV	203	95	0.02%	0.002%
89	10.298	2836	2838	2842	rVB2	191	126	0.02%	0.003%
90	10.318	2842	2844	2847	rBV	186	88	0.01%	0.002%
91	10.433	2867	2880	2903	rVB	179414	291784	48.05%	6.395%
92	10.568	2920	2922	2927	rBV	190	215	0.04%	0.005%
93	10.607	2928	2934	2942	rVV	1021	1477	0.24%	0.032%
94	10.945	3036	3039	3046	rBV	255	236	0.04%	0.005%
95	11.041	3066	3069	3071	rBV	219	143	0.02%	0.003%
96	11.128	3091	3096	3102	rBV2	271	332	0.05%	0.007%
97	11.485	3195	3207	3231	rBV	227924	361623	59.55%	7.925%
98	11.861	3312	3324	3342	rBV	220556	350243	57.67%	7.676%
99	12.353	3475	3477	3479	rBV	169	67	0.01%	0.001%
100	12.485	3511	3518	3522	rBV2	387	525	0.09%	0.012%


Sum of corrected areas: 4562829

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027640.D
Acq On : 12 Oct 2018 22:00
Operator : MD/SY
Sample : J5405-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08Y0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

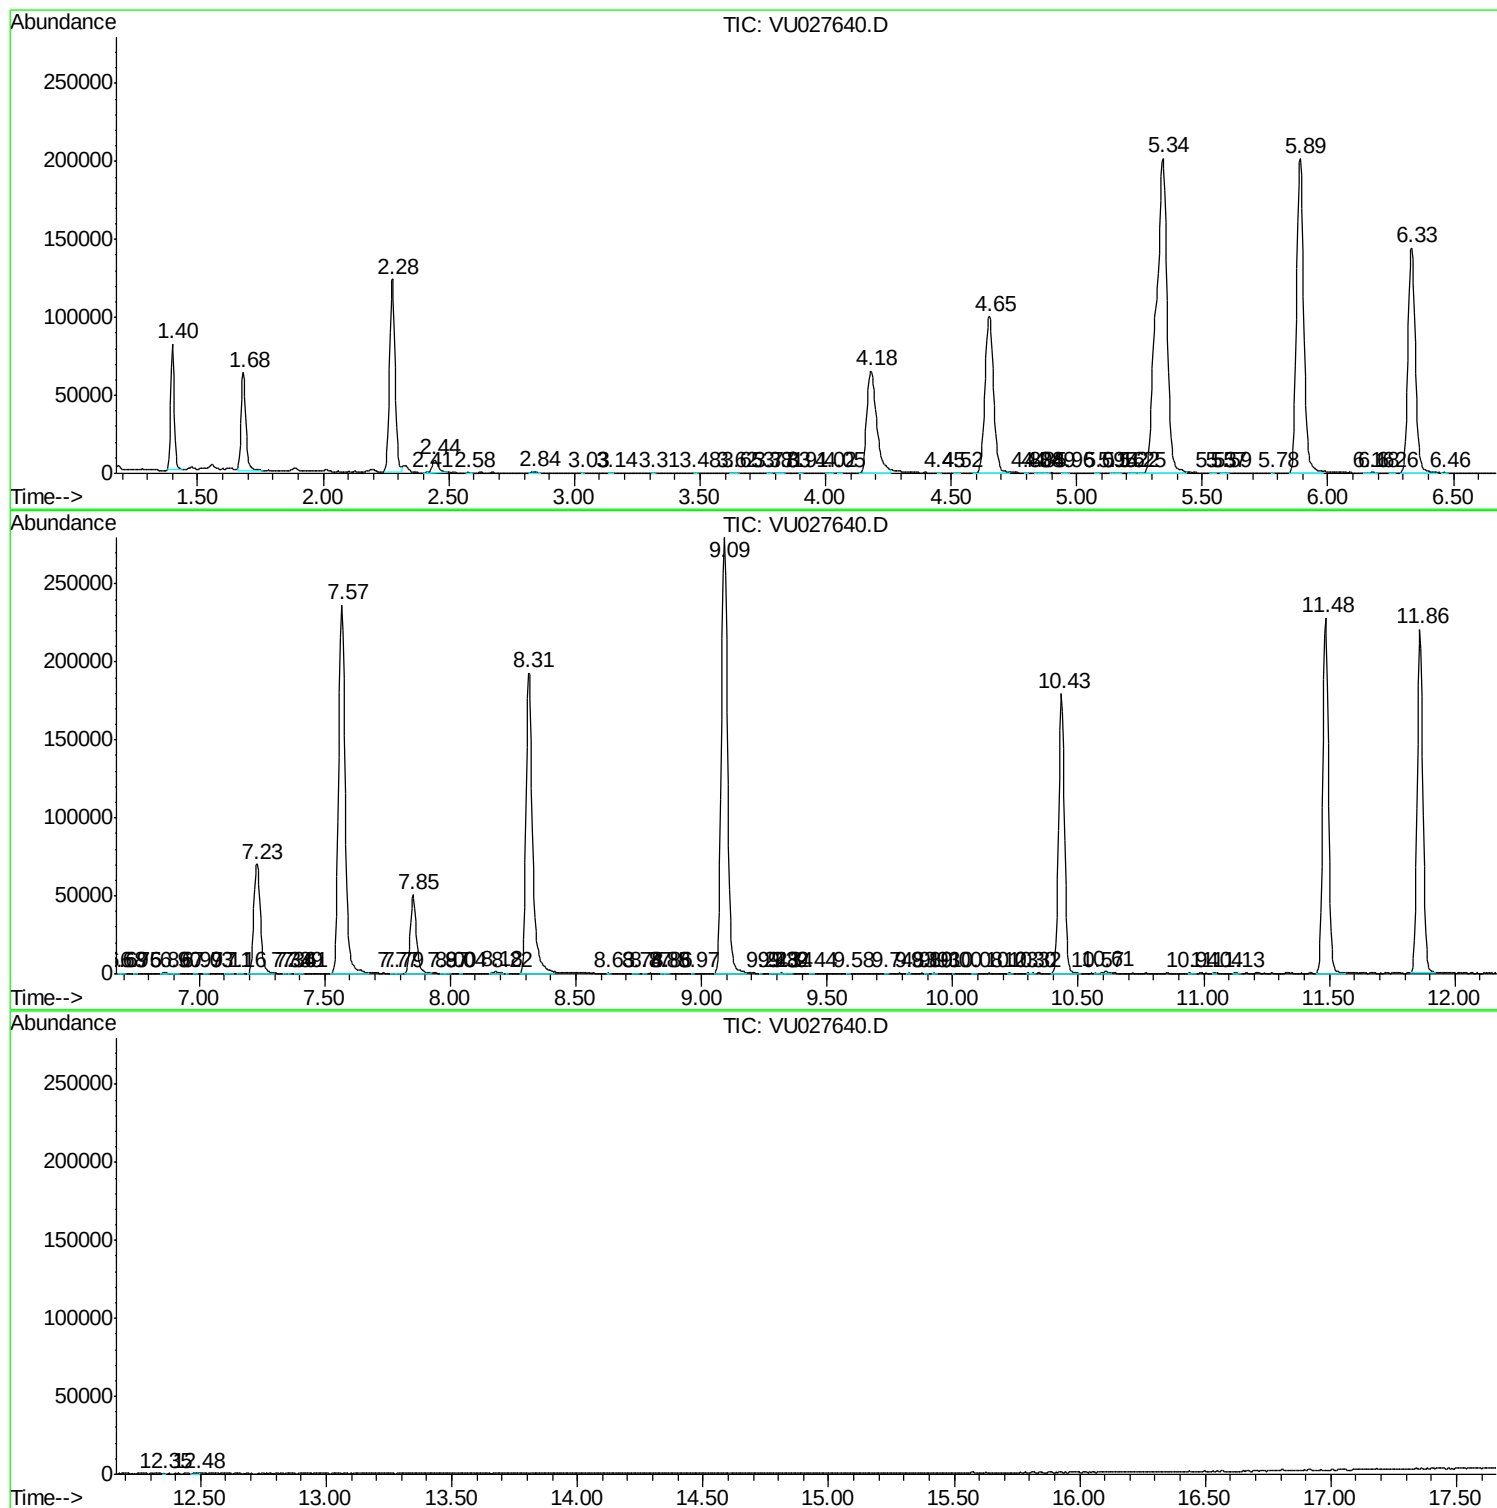

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027640.D
Acq On : 12 Oct 2018 22:00
Operator : MD/SY
Sample : J5405-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08Y0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027640.D
Acq On : 12 Oct 2018 22:00
Operator : MD/SY
Sample : J5405-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08Y0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc