

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
 Data File : VU027641.D
 Acq On : 12 Oct 2018 22:23
 Operator : MD/SY
 Sample : J5405-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08Y1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.398	64	70	84	rBV	82717	85102	13.75%	1.779%
2	1.681	151	158	175	rVB	65635	83595	13.51%	1.747%
3	2.273	331	342	354	rBV	126762	194111	31.36%	4.057%
4	2.443	385	395	411	rBV	6029	10432	1.69%	0.218%
5	2.620	445	450	456	rBV2	228	317	0.05%	0.007%
6	2.845	516	520	525	rVB3	365	406	0.07%	0.008%
7	2.929	544	546	550	rBV2	143	92	0.01%	0.002%
8	3.048	580	583	587	rVB2	181	138	0.02%	0.003%
9	3.196	625	629	630	rBV2	159	82	0.01%	0.002%
10	3.331	668	671	674	rBV	206	84	0.01%	0.002%
11	3.395	687	691	693	rVB	119	67	0.01%	0.001%
12	3.517	727	729	732	rVV	191	105	0.02%	0.002%
13	3.646	764	769	773	rVB	142	132	0.02%	0.003%
14	3.668	773	776	780	rBV	183	94	0.02%	0.002%
15	3.733	794	796	799	rVB	149	63	0.01%	0.001%
16	3.774	804	809	812	rVB2	195	157	0.03%	0.003%
17	3.797	812	816	818	rBV	84	72	0.01%	0.002%
18	3.813	819	821	823	rBV	144	58	0.01%	0.001%
19	3.871	834	839	840	rBV	203	100	0.02%	0.002%
20	3.919	849	854	859	rBV	104	114	0.02%	0.002%
21	3.951	859	864	870	rBV	152	161	0.03%	0.003%
22	4.022	884	886	890	rVB	158	77	0.01%	0.002%
23	4.045	890	893	898	rBV	122	105	0.02%	0.002%
24	4.180	921	935	965	rBV	65516	174059	28.12%	3.638%
25	4.491	1030	1032	1034	rBV	137	83	0.01%	0.002%
26	4.546	1045	1049	1053	rBV	103	83	0.01%	0.002%
27	4.588	1059	1062	1064	rBV	83	57	0.01%	0.001%
28	4.652	1064	1082	1108	rBV	104111	247017	39.91%	5.163%
29	4.794	1121	1126	1129	rVB	68	66	0.01%	0.001%
30	4.813	1129	1132	1135	rBV	142	100	0.02%	0.002%
31	4.945	1168	1173	1175	rBV	106	102	0.02%	0.002%
32	5.221	1257	1259	1263	rVB	160	55	0.01%	0.001%
33	5.250	1263	1268	1271	rBV	98	75	0.01%	0.002%
34	5.343	1273	1297	1318	rBV2	208065	618944	100.00%	12.937%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
 Data File : VU027641.D
 Acq On : 12 Oct 2018 22:23
 Operator : MD/SY
 Sample : J5405-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08Y1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

35	5.504	1343	1347	1350	rBV3	551	449	0.07%	0.009%
36	5.594	1371	1375	1379	rBV	168	224	0.04%	0.005%
37	5.649	1388	1392	1396	rVB2	242	248	0.04%	0.005%
38	5.681	1396	1402	1409	rVB	210	192	0.03%	0.004%
39	5.716	1409	1413	1417	rBV	218	214	0.03%	0.004%
40	5.755	1422	1425	1426	rBV	169	100	0.02%	0.002%
41	5.794	1432	1437	1439	rBV2	284	278	0.04%	0.006%
42	5.835	1448	1450	1453	rBV	135	75	0.01%	0.002%
43	5.890	1453	1467	1495	rBV	222831	445298	71.94%	9.308%
44	6.112	1532	1536	1539	rBV2	133	89	0.01%	0.002%
45	6.131	1539	1542	1543	rBV	143	99	0.02%	0.002%
46	6.176	1552	1556	1565	rBV5	536	692	0.11%	0.014%
47	6.334	1591	1605	1627	rBV	147442	296661	47.93%	6.201%
48	6.466	1641	1646	1650	rVB3	324	388	0.06%	0.008%
49	6.581	1680	1682	1685	rVB2	184	100	0.02%	0.002%
50	6.601	1685	1688	1690	rBV	153	108	0.02%	0.002%
51	6.646	1699	1702	1704	rVB2	133	74	0.01%	0.002%
52	6.659	1704	1706	1710	rVB	170	87	0.01%	0.002%
53	6.681	1711	1713	1715	rBV	153	66	0.01%	0.001%
54	6.742	1730	1732	1734	rVB	139	61	0.01%	0.001%
55	6.800	1748	1750	1753	rVB	200	92	0.01%	0.002%
56	6.823	1753	1757	1758	rBV	97	67	0.01%	0.001%
57	6.861	1765	1769	1770	rBV	425	301	0.05%	0.006%
58	6.896	1777	1780	1784	rVB	133	100	0.02%	0.002%
59	6.948	1792	1796	1797	rBV	111	70	0.01%	0.001%
60	7.077	1834	1836	1840	rBV	152	91	0.01%	0.002%
61	7.102	1842	1844	1847	rVB	149	63	0.01%	0.001%
62	7.147	1854	1858	1862	rBV2	160	126	0.02%	0.003%
63	7.231	1872	1884	1909	rBV	73169	131637	21.27%	2.752%
64	7.340	1914	1918	1920	rVB	243	147	0.02%	0.003%
65	7.366	1922	1926	1928	rBV	271	163	0.03%	0.003%
66	7.405	1936	1938	1940	rBV	129	75	0.01%	0.002%
67	7.511	1968	1971	1973	rBV	159	69	0.01%	0.001%
68	7.568	1975	1989	2018	rBV	241534	436385	70.50%	9.121%
69	7.774	2050	2053	2054	rBV	154	72	0.01%	0.002%
70	7.803	2058	2062	2064	rBV2	181	149	0.02%	0.003%
71	7.851	2064	2077	2096	rBV	51256	88023	14.22%	1.840%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
 Data File : VU027641.D
 Acq On : 12 Oct 2018 22:23
 Operator : MD/SY
 Sample : J5405-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08Y1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

72	7.954	2106	2109	2110	rBV	233	121	0.02%	0.003%
73	7.999	2122	2123	2128	rBV	333	195	0.03%	0.004%
74	8.051	2136	2139	2142	rBV	229	150	0.02%	0.003%
75	8.080	2145	2148	2151	rVV	216	144	0.02%	0.003%
76	8.102	2151	2155	2158	rVB2	170	141	0.02%	0.003%
77	8.157	2169	2172	2173	rBV	306	172	0.03%	0.004%
78	8.240	2193	2198	2200	rBV	208	131	0.02%	0.003%
79	8.266	2203	2206	2209	rVB	172	72	0.01%	0.002%
80	8.311	2209	2220	2258	rBV	198507	360412	58.23%	7.533%
81	8.581	2302	2304	2305	rVB	217	69	0.01%	0.001%
82	8.755	2355	2358	2359	rBV	142	87	0.01%	0.002%
83	8.803	2371	2373	2377	rBV2	177	141	0.02%	0.003%
84	9.006	2433	2436	2440	rVB	186	100	0.02%	0.002%
85	9.044	2446	2448	2450	rBV	150	105	0.02%	0.002%
86	9.093	2450	2463	2493	rVV	313070	527757	85.27%	11.031%
87	9.253	2510	2513	2517	rVB2	256	201	0.03%	0.004%
88	9.385	2551	2554	2556	rBV	187	111	0.02%	0.002%
89	9.430	2564	2568	2572	rBV	166	158	0.03%	0.003%
90	9.507	2589	2592	2597	rBV	170	160	0.03%	0.003%
91	9.655	2635	2638	2641	rBV	144	92	0.01%	0.002%
92	10.359	2855	2857	2861	rBV	208	133	0.02%	0.003%
93	10.388	2864	2866	2868	rVV	184	90	0.01%	0.002%
94	10.433	2868	2880	2904	rVV	187173	298574	48.24%	6.241%
95	10.729	2971	2972	2977	rBV	135	74	0.01%	0.002%
96	11.199	3115	3118	3123	rVB	236	189	0.03%	0.004%
97	11.227	3124	3127	3135	rBV	322	347	0.06%	0.007%
98	11.485	3195	3207	3231	rBV	260502	410871	66.38%	8.588%
99	11.684	3266	3269	3272	rBV	184	143	0.02%	0.003%
100	11.861	3312	3324	3347	rBV	225889	363794	58.78%	7.604%


Sum of corrected areas: 4784172

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027641.D
Acq On : 12 Oct 2018 22:23
Operator : MD/SY
Sample : J5405-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08Y1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

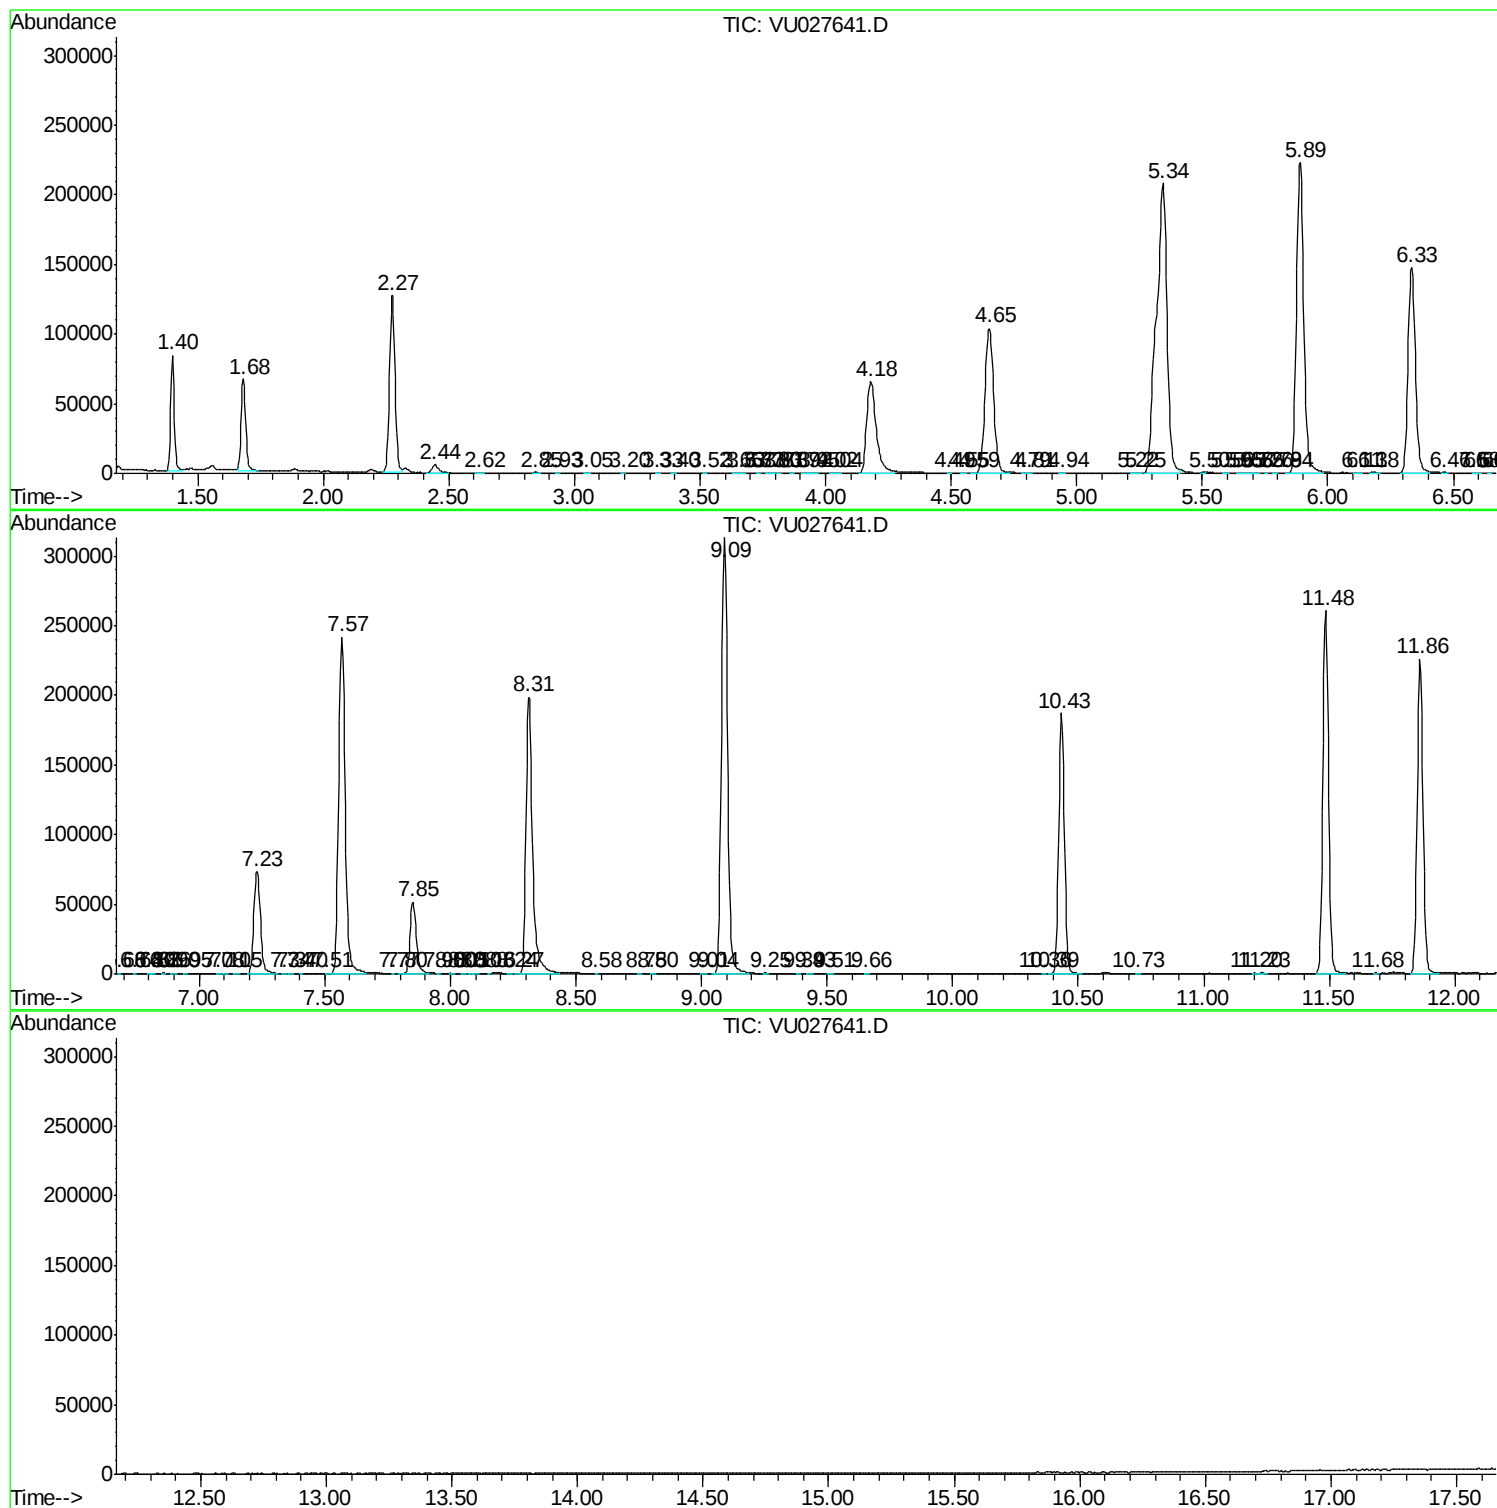

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027641.D
Acq On : 12 Oct 2018 22:23
Operator : MD/SY
Sample : J5405-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08Y1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027641.D
Acq On : 12 Oct 2018 22:23
Operator : MD/SY
Sample : J5405-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08Y1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc