

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
 Data File : VU027644.D
 Acq On : 12 Oct 2018 23:32
 Operator : MD/SY
 Sample : J5405-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08Y4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.398	64	70	81	rBV	80833	83620	13.85%	1.835%
2	1.681	151	158	171	rVB	62066	78695	13.04%	1.727%
3	2.276	332	343	355	rBV	122204	187549	31.07%	4.116%
4	2.443	386	395	410	rBV	11074	18792	3.11%	0.412%
5	2.549	426	428	430	rBV	174	87	0.01%	0.002%
6	2.839	511	518	521	rBV2	667	897	0.15%	0.020%
7	3.070	588	590	591	rBV2	159	49	0.01%	0.001%
8	3.125	604	607	609	rBV	118	86	0.01%	0.002%
9	3.241	640	643	644	rBV	200	88	0.01%	0.002%
10	3.295	657	660	663	rBV	197	95	0.02%	0.002%
11	3.318	664	667	675	rBV	115	125	0.02%	0.003%
12	3.360	679	680	684	rVB	144	59	0.01%	0.001%
13	3.511	724	727	731	rBV	79	63	0.01%	0.001%
14	3.591	749	752	754	rBV	96	47	0.01%	0.001%
15	3.630	759	764	767	rBV	143	134	0.02%	0.003%
16	3.665	773	775	777	rBV	148	89	0.01%	0.002%
17	3.758	800	804	809	rVB	122	121	0.02%	0.003%
18	3.781	809	811	815	rBV	80	65	0.01%	0.001%
19	3.823	820	824	825	rBV	158	105	0.02%	0.002%
20	3.861	832	836	838	rBV	131	105	0.02%	0.002%
21	3.910	848	851	854	rBV	100	74	0.01%	0.002%
22	4.180	921	935	967	rBV	65120	179491	29.74%	3.940%
23	4.440	1012	1016	1018	rBV	193	150	0.02%	0.003%
24	4.495	1031	1033	1035	rVB	143	59	0.01%	0.001%
25	4.508	1035	1037	1039	rBV	134	56	0.01%	0.001%
26	4.556	1050	1052	1053	rBV	117	46	0.01%	0.001%
27	4.652	1064	1082	1109	rBV	100592	236986	39.26%	5.202%
28	4.807	1128	1130	1134	rVV	145	127	0.02%	0.003%
29	4.897	1148	1158	1162	rBV2	429	595	0.10%	0.013%
30	4.942	1169	1172	1175	rBV	94	74	0.01%	0.002%
31	4.958	1175	1177	1179	rVB	144	61	0.01%	0.001%
32	5.176	1243	1245	1251	rVB2	192	132	0.02%	0.003%
33	5.212	1254	1256	1259	rBV	66	46	0.01%	0.001%
34	5.244	1263	1266	1269	rBV	68	57	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
 Data File : VU027644.D
 Acq On : 12 Oct 2018 23:32
 Operator : MD/SY
 Sample : J5405-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08Y4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

35	5.344	1273	1297	1322	rBV2	200494	603602	100.00%	13.248%
36	5.553	1360	1362	1364	rVB	113	46	0.01%	0.001%
37	5.623	1381	1384	1387	rBV	109	67	0.01%	0.001%
38	5.643	1387	1390	1392	rBV	79	47	0.01%	0.001%
39	5.813	1439	1443	1446	rBV	100	73	0.01%	0.002%
40	5.890	1451	1467	1506	rBV	214968	431813	71.54%	9.478%
41	6.122	1537	1539	1540	rBV	159	49	0.01%	0.001%
42	6.180	1552	1557	1563	rBV4	502	591	0.10%	0.013%
43	6.234	1569	1574	1577	rBV	499	489	0.08%	0.011%
44	6.334	1590	1605	1630	rBV	143584	287603	47.65%	6.313%
45	6.533	1665	1667	1669	rBV	133	56	0.01%	0.001%
46	6.543	1669	1670	1673	rVB	128	48	0.01%	0.001%
47	6.569	1673	1678	1681	rBV2	218	211	0.03%	0.005%
48	6.626	1694	1696	1697	rVB2	106	40	0.01%	0.001%
49	6.688	1711	1715	1718	rBV2	250	178	0.03%	0.004%
50	6.720	1723	1725	1728	rBV2	137	82	0.01%	0.002%
51	6.749	1732	1734	1737	rVB	153	67	0.01%	0.001%
52	6.771	1740	1741	1744	rVB	137	53	0.01%	0.001%
53	6.832	1756	1760	1763	rBV	67	63	0.01%	0.001%
54	6.861	1763	1769	1770	rBV2	452	427	0.07%	0.009%
55	6.893	1777	1779	1780	rBV	153	64	0.01%	0.001%
56	7.006	1812	1814	1821	rVB2	147	105	0.02%	0.002%
57	7.231	1872	1884	1908	rBV	68878	125561	20.80%	2.756%
58	7.350	1919	1921	1925	rVB	240	111	0.02%	0.002%
59	7.382	1929	1931	1933	rBV	153	105	0.02%	0.002%
60	7.417	1940	1942	1944	rBV2	148	84	0.01%	0.002%
61	7.459	1951	1955	1956	rBV	124	108	0.02%	0.002%
62	7.569	1975	1989	2009	rBV	233539	416158	68.95%	9.134%
63	7.852	2066	2077	2098	rBV2	50397	86096	14.26%	1.890%
64	8.054	2131	2140	2144	rBV	158	218	0.04%	0.005%
65	8.070	2144	2145	2147	rVB	123	42	0.01%	0.001%
66	8.089	2148	2151	2154	rVV	205	129	0.02%	0.003%
67	8.186	2169	2181	2185	rBV2	1133	1592	0.26%	0.035%
68	8.247	2197	2200	2202	rVB	148	81	0.01%	0.002%
69	8.315	2208	2221	2251	rBV	186683	340994	56.49%	7.484%
70	8.549	2291	2294	2297	rBV2	246	158	0.03%	0.003%
71	8.639	2319	2322	2325	rBV	176	79	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
 Data File : VU027644.D
 Acq On : 12 Oct 2018 23:32
 Operator : MD/SY
 Sample : J5405-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08Y4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

72	8.668	2329	2331	2334	rVB	169	87	0.01%	0.002%
73	8.691	2334	2338	2342	rBV	192	177	0.03%	0.004%
74	8.781	2364	2366	2370	rBV	253	181	0.03%	0.004%
75	8.842	2381	2385	2387	rBV2	127	84	0.01%	0.002%
76	8.996	2430	2433	2434	rBV	154	67	0.01%	0.001%
77	9.089	2449	2462	2490	rBV	299134	502336	83.22%	11.026%
78	9.273	2517	2519	2520	rBV	184	96	0.02%	0.002%
79	9.318	2531	2533	2538	rVB2	185	122	0.02%	0.003%
80	9.343	2539	2541	2542	rBV	143	80	0.01%	0.002%
81	9.388	2550	2555	2560	rBV2	202	250	0.04%	0.005%
82	9.408	2560	2561	2564	rVB2	148	56	0.01%	0.001%
83	9.446	2571	2573	2575	rBV	128	73	0.01%	0.002%
84	9.485	2583	2585	2590	rVB	207	107	0.02%	0.002%
85	9.597	2614	2620	2623	rBV	190	187	0.03%	0.004%
86	9.614	2623	2625	2627	rBV	137	79	0.01%	0.002%
87	9.739	2661	2664	2665	rBV	159	73	0.01%	0.002%
88	9.768	2670	2673	2678	rVB2	229	187	0.03%	0.004%
89	9.832	2692	2693	2696	rVB	158	41	0.01%	0.001%
90	9.858	2699	2701	2702	rBV	122	49	0.01%	0.001%
91	10.028	2752	2754	2757	rBV	228	153	0.03%	0.003%
92	10.138	2785	2788	2789	rBV	178	84	0.01%	0.002%
93	10.192	2802	2805	2807	rBV	151	118	0.02%	0.003%
94	10.433	2867	2880	2896	rBV	178675	287572	47.64%	6.312%
95	10.607	2928	2934	2942	rVB5	1033	1557	0.26%	0.034%
96	11.093	3082	3085	3089	rVB	240	145	0.02%	0.003%
97	11.485	3195	3207	3233	rBV	232287	362792	60.10%	7.963%
98	11.861	3312	3324	3348	rBV	191185	312887	51.84%	6.867%
99	12.070	3385	3389	3391	rBV2	260	184	0.03%	0.004%
100	13.382	3795	3797	3799	rBV	299	131	0.02%	0.003%


Sum of corrected areas: 4556070

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027644.D
Acq On : 12 Oct 2018 23:32
Operator : MD/SY
Sample : J5405-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08Y4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

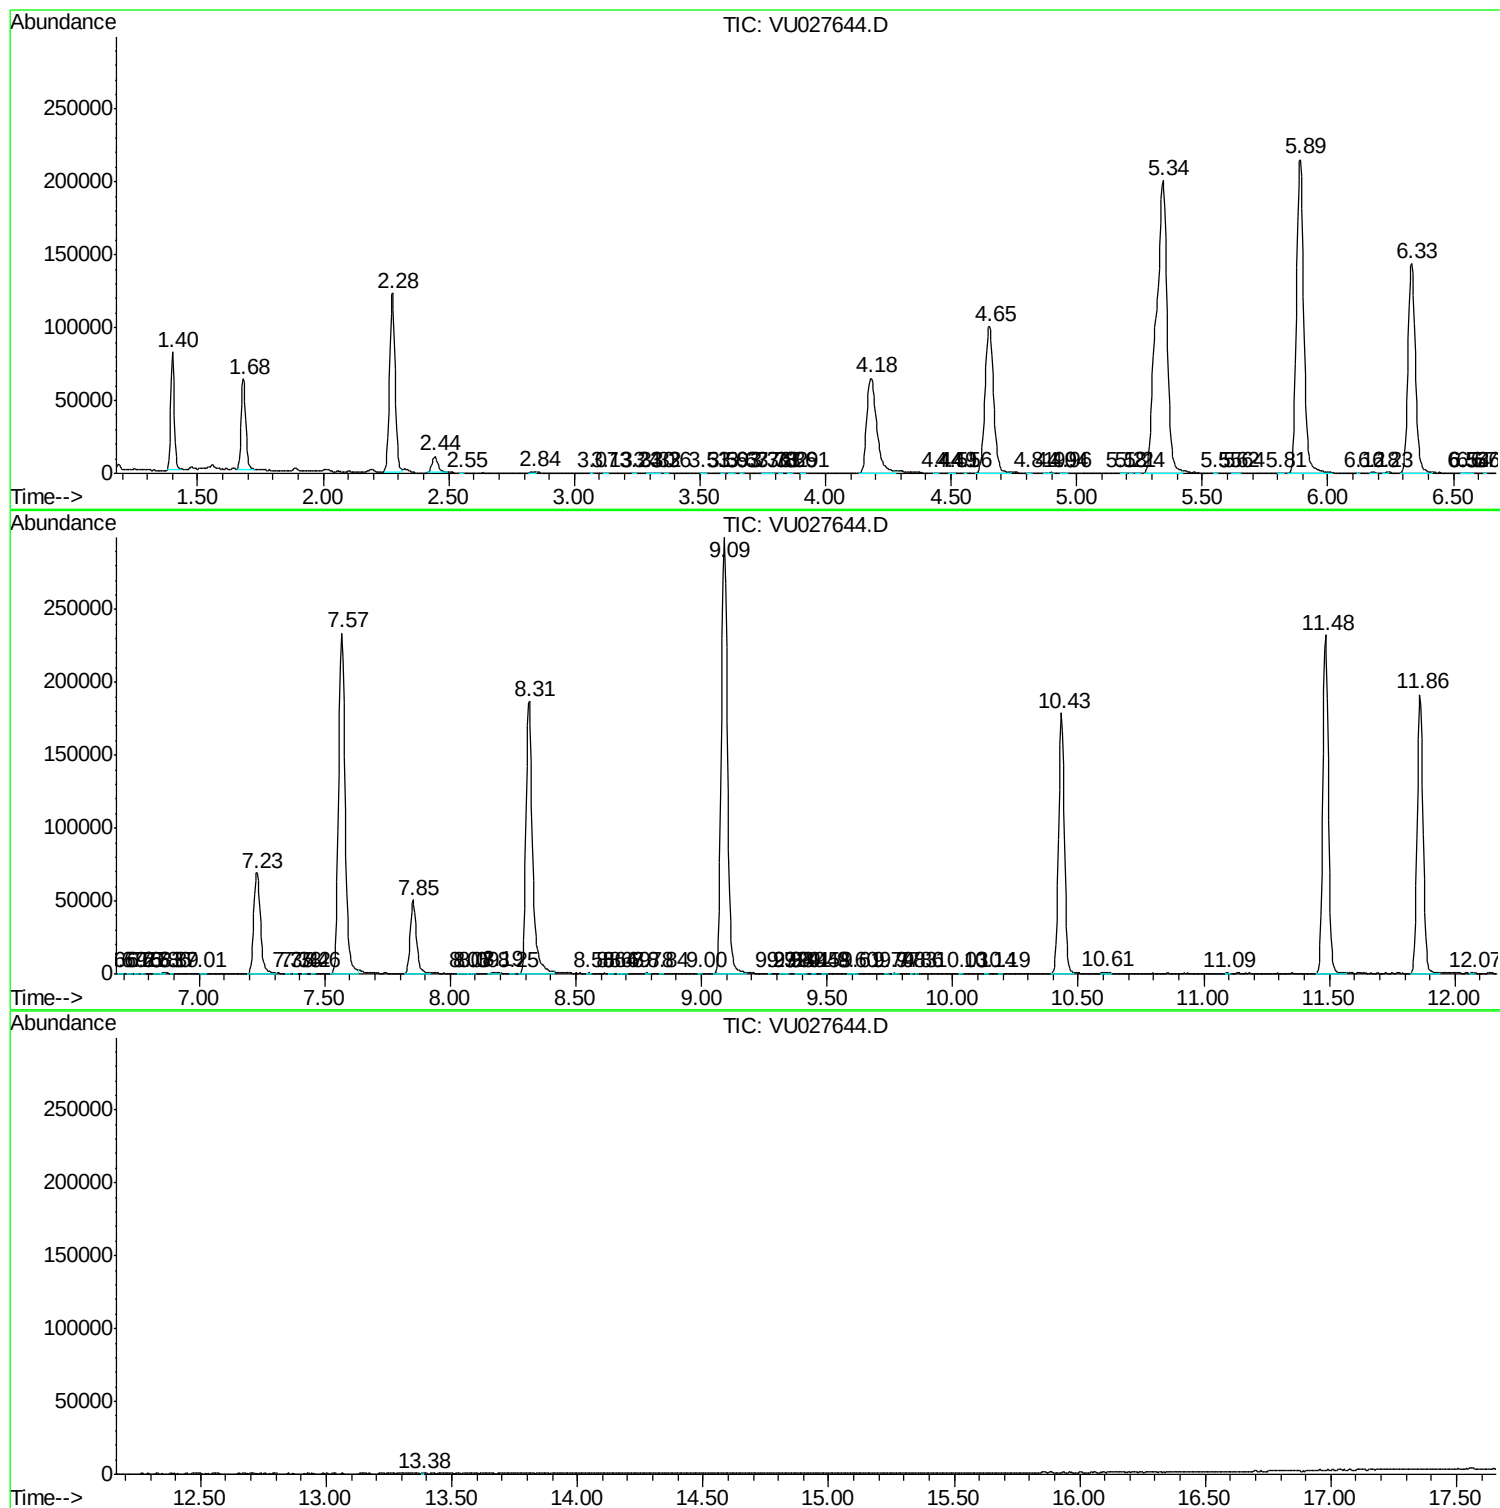

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027644.D
Acq On : 12 Oct 2018 23:32
Operator : MD/SY
Sample : J5405-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08Y4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027644.D
Acq On : 12 Oct 2018 23:32
Operator : MD/SY
Sample : J5405-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08Y4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc
