

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
 Data File : VU027647.D
 Acq On : 13 Oct 2018 00:41
 Operator : MD/SY
 Sample : J5405-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08Y7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.399	64	70	82	rBV	78791	82127	13.73%	1.727%
2	1.681	151	158	170	rVB	64510	79419	13.27%	1.670%
3	2.273	332	342	354	rBV	123291	189211	31.62%	3.980%
4	2.443	385	395	408	rBV	8445	14814	2.48%	0.312%
5	2.604	443	445	447	rVB	160	65	0.01%	0.001%
6	2.624	447	451	452	rBV	151	105	0.02%	0.002%
7	2.839	511	518	526	rBV2	729	1302	0.22%	0.027%
8	3.016	567	573	577	rBV2	200	262	0.04%	0.006%
9	3.048	581	583	585	rVB	145	38	0.01%	0.001%
10	3.138	608	611	614	rBV	92	77	0.01%	0.002%
11	3.177	621	623	627	rBV2	136	97	0.02%	0.002%
12	3.231	638	640	643	rBV	115	69	0.01%	0.001%
13	3.321	666	668	671	rBV	156	52	0.01%	0.001%
14	3.395	690	691	693	rVB	141	51	0.01%	0.001%
15	3.415	693	697	700	rBV2	220	157	0.03%	0.003%
16	3.431	700	702	704	rVV2	131	60	0.01%	0.001%
17	3.533	731	734	737	rVB	141	61	0.01%	0.001%
18	3.607	755	757	758	rBV	157	49	0.01%	0.001%
19	3.678	777	779	781	rBV	144	77	0.01%	0.002%
20	3.871	836	839	841	rBV	80	58	0.01%	0.001%
21	3.935	857	859	862	rBV	150	61	0.01%	0.001%
22	4.019	880	885	887	rBV	178	124	0.02%	0.003%
23	4.083	902	905	908	rVB	143	80	0.01%	0.002%
24	4.125	913	918	921	rBV	221	153	0.03%	0.003%
25	4.180	921	935	968	rBV	63004	175146	29.27%	3.684%
26	4.479	1026	1028	1032	rVB	277	103	0.02%	0.002%
27	4.501	1032	1035	1038	rBV	79	52	0.01%	0.001%
28	4.517	1038	1040	1044	rVV	136	70	0.01%	0.001%
29	4.550	1049	1050	1053	rVB	151	55	0.01%	0.001%
30	4.569	1053	1056	1057	rBV	69	41	0.01%	0.001%
31	4.652	1064	1082	1111	rBV	99361	236642	39.55%	4.977%
32	4.826	1134	1136	1139	rVB	180	86	0.01%	0.002%
33	4.868	1145	1149	1153	rBV	126	103	0.02%	0.002%
34	4.890	1153	1156	1159	rBV	448	289	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
 Data File : VU027647.D
 Acq On : 13 Oct 2018 00:41
 Operator : MD/SY
 Sample : J5405-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08Y7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

35	4.906	1159	1161	1165	rVV	68	37	0.01%	0.001%
36	4.951	1172	1175	1180	rBV	74	90	0.02%	0.002%
37	5.051	1203	1206	1209	rBV	121	84	0.01%	0.002%
38	5.151	1234	1237	1240	rBV	81	60	0.01%	0.001%
39	5.215	1253	1257	1260	rBV	94	71	0.01%	0.001%
40	5.241	1260	1265	1268	rBV	58	60	0.01%	0.001%
41	5.260	1268	1271	1273	rBV	59	42	0.01%	0.001%
42	5.344	1273	1297	1326	rBV2	200068	598350	100.00%	12.585%
43	5.549	1359	1361	1362	rVB2	105	40	0.01%	0.001%
44	5.720	1411	1414	1418	rVB	121	99	0.02%	0.002%
45	5.742	1418	1421	1423	rBV	108	77	0.01%	0.002%
46	5.781	1431	1433	1437	rVB	96	65	0.01%	0.001%
47	5.890	1451	1467	1501	rBV	221015	438711	73.32%	9.227%
48	6.112	1533	1536	1540	rBV	186	121	0.02%	0.003%
49	6.167	1551	1553	1555	rBV2	304	211	0.04%	0.004%
50	6.176	1555	1556	1564	rVB3	506	480	0.08%	0.010%
51	6.334	1591	1605	1638	rBV	144333	289847	48.44%	6.096%
52	6.450	1639	1641	1642	rBV	173	72	0.01%	0.002%
53	6.569	1674	1678	1680	rBV	75	63	0.01%	0.001%
54	6.684	1711	1714	1717	rBV	90	47	0.01%	0.001%
55	6.823	1754	1757	1760	rBV	85	55	0.01%	0.001%
56	6.865	1765	1770	1776	rVB3	319	334	0.06%	0.007%
57	6.971	1800	1803	1807	rBV	113	87	0.01%	0.002%
58	7.057	1828	1830	1831	rBV	149	64	0.01%	0.001%
59	7.144	1854	1857	1860	rBV	71	58	0.01%	0.001%
60	7.231	1872	1884	1902	rBV	67862	122168	20.42%	2.569%
61	7.331	1913	1915	1917	rBV2	122	67	0.01%	0.001%
62	7.382	1929	1931	1932	rVB	118	45	0.01%	0.001%
63	7.392	1932	1934	1938	rVB	114	62	0.01%	0.001%
64	7.414	1938	1941	1944	rBV	67	54	0.01%	0.001%
65	7.472	1955	1959	1962	rBV	263	180	0.03%	0.004%
66	7.569	1975	1989	2007	rBV	235567	419523	70.11%	8.823%
67	7.762	2046	2049	2051	rBV	185	153	0.03%	0.003%
68	7.852	2066	2077	2099	rBV	49616	84654	14.15%	1.780%
69	8.006	2123	2125	2129	rVB2	200	110	0.02%	0.002%
70	8.038	2133	2135	2139	rVB	182	73	0.01%	0.002%
71	8.067	2139	2144	2147	rBV	98	83	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
 Data File : VU027647.D
 Acq On : 13 Oct 2018 00:41
 Operator : MD/SY
 Sample : J5405-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08Y7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

72	8.086	2147	2150	2153	rBV	89	67	0.01%	0.001%
73	8.180	2171	2179	2184	rBV3	869	1404	0.23%	0.030%
74	8.228	2184	2194	2209	rVV	61989	106488	17.80%	2.240%
75	8.311	2209	2220	2254	rVV	192642	343364	57.39%	7.222%
76	8.655	2322	2327	2331	rBV	104	131	0.02%	0.003%
77	8.678	2331	2334	2335	rBV	121	54	0.01%	0.001%
78	8.742	2352	2354	2357	rBV2	140	85	0.01%	0.002%
79	8.797	2369	2371	2372	rBV2	103	44	0.01%	0.001%
80	8.929	2408	2412	2414	rBV2	112	72	0.01%	0.002%
81	8.977	2425	2427	2429	rBV2	104	50	0.01%	0.001%
82	9.090	2450	2462	2490	rBV	308895	520686	87.02%	10.951%
83	9.308	2526	2530	2531	rBV	252	212	0.04%	0.004%
84	9.417	2562	2564	2568	rBV	119	64	0.01%	0.001%
85	9.459	2575	2577	2579	rBV	125	54	0.01%	0.001%
86	9.636	2628	2632	2636	rBV2	172	139	0.02%	0.003%
87	9.655	2636	2638	2639	rBV	111	61	0.01%	0.001%
88	9.784	2675	2678	2680	rBV2	163	114	0.02%	0.002%
89	10.028	2751	2754	2757	rBV	170	106	0.02%	0.002%
90	10.048	2757	2760	2765	rVB2	167	172	0.03%	0.004%
91	10.192	2803	2805	2807	rBV	149	89	0.01%	0.002%
92	10.234	2815	2818	2821	rBV2	170	143	0.02%	0.003%
93	10.266	2826	2828	2831	rVB	198	117	0.02%	0.002%
94	10.434	2868	2880	2901	rBV	181485	290039	48.47%	6.100%
95	10.707	2962	2965	2968	rBV	242	151	0.03%	0.003%
96	10.781	2985	2988	2997	rVB2	315	296	0.05%	0.006%
97	10.919	3029	3031	3033	rBV	145	38	0.01%	0.001%
98	11.485	3196	3207	3229	rBV	261240	407021	68.02%	8.561%
99	11.861	3312	3324	3348	rBV	216636	345447	57.73%	7.266%
100	14.240	4060	4064	4066	rBV2	457	352	0.06%	0.007%


Sum of corrected areas: 4754613

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027647.D
Acq On : 13 Oct 2018 00:41
Operator : MD/SY
Sample : J5405-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08Y7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

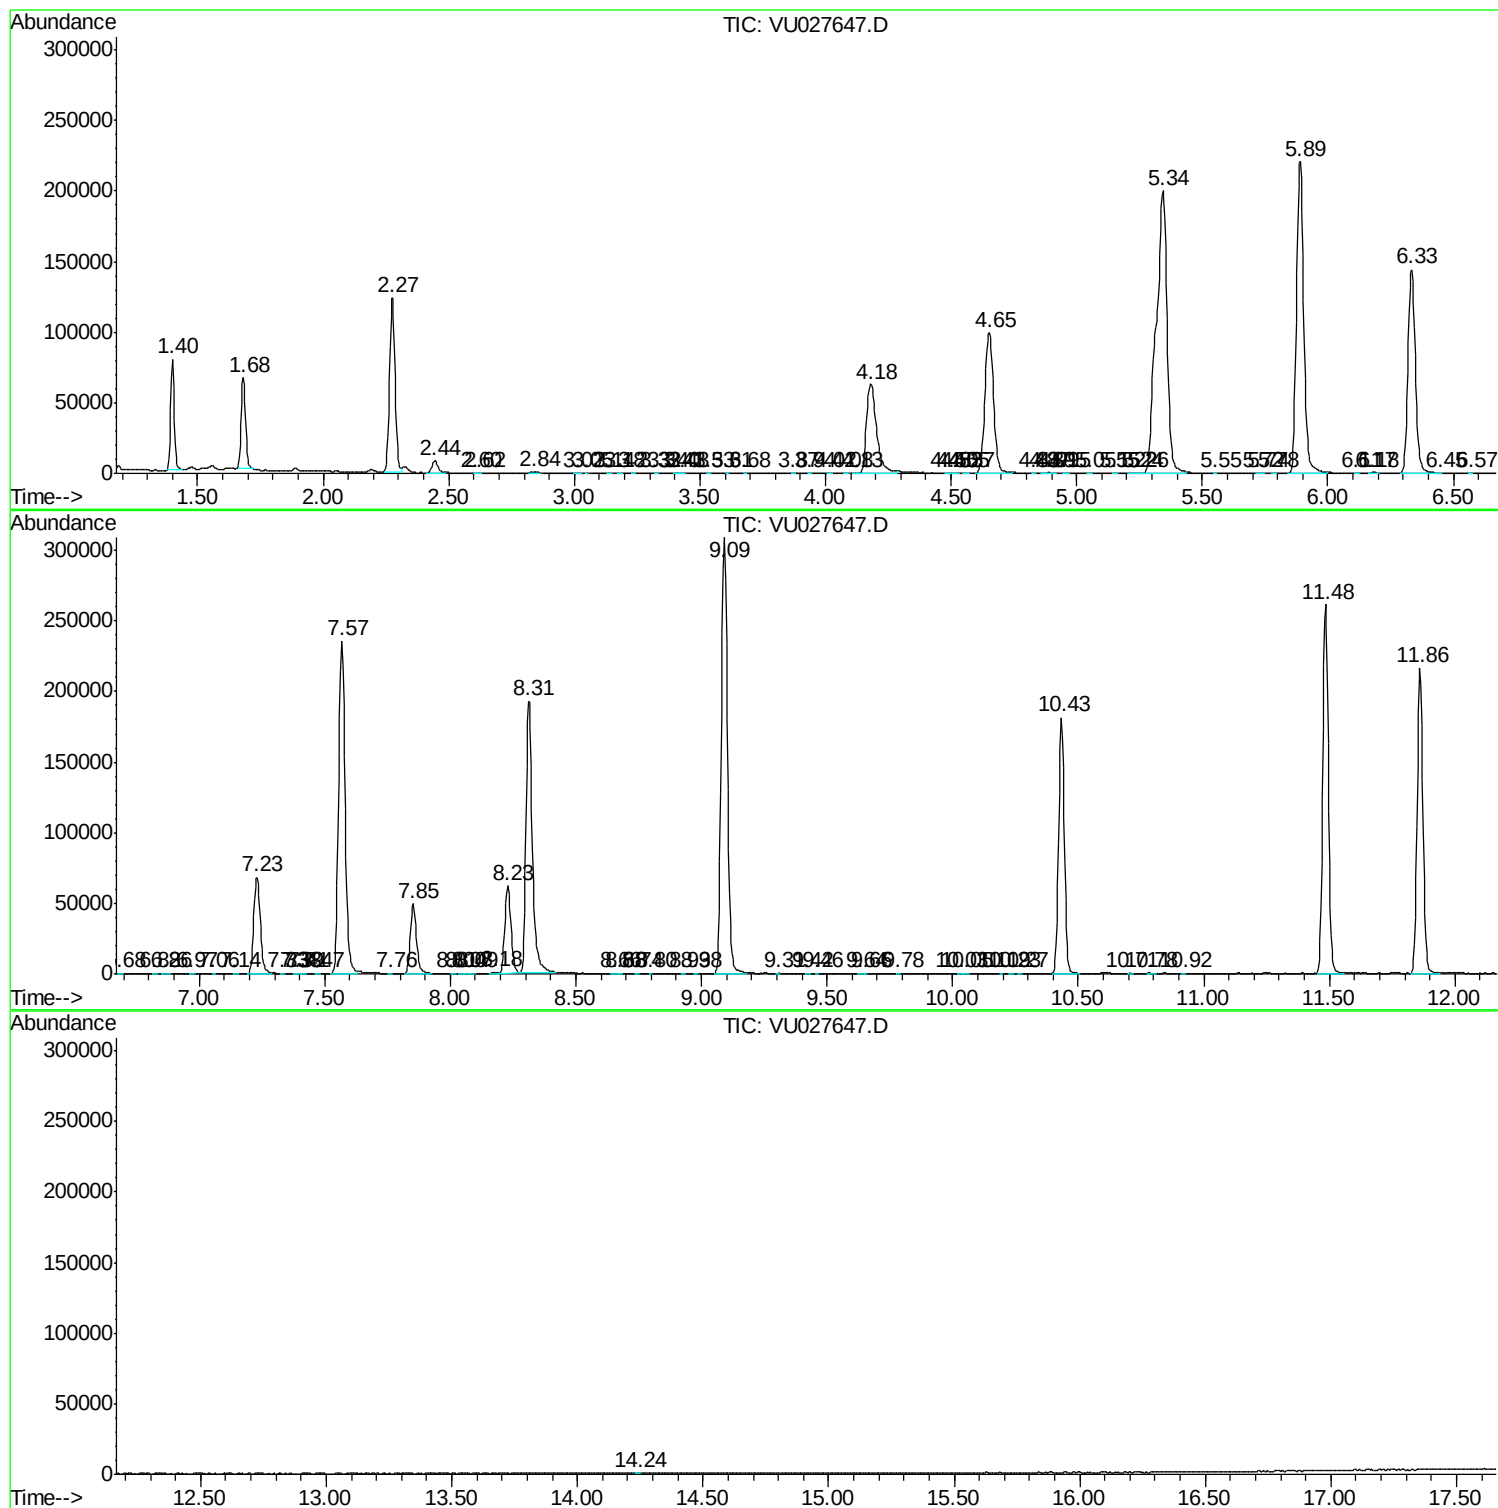

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027647.D
Acq On : 13 Oct 2018 00:41
Operator : MD/SY
Sample : J5405-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08Y7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101218\
Data File : VU027647.D
Acq On : 13 Oct 2018 00:41
Operator : MD/SY
Sample : J5405-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08Y7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc