


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101218\
 Data File : VU027610.D
 Acq On : 12 Oct 2018 08:13
 Operator : MD/SY
 Sample : BFB42
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB42

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis
 Last Update : Sat Oct 13 04:07:45 2018

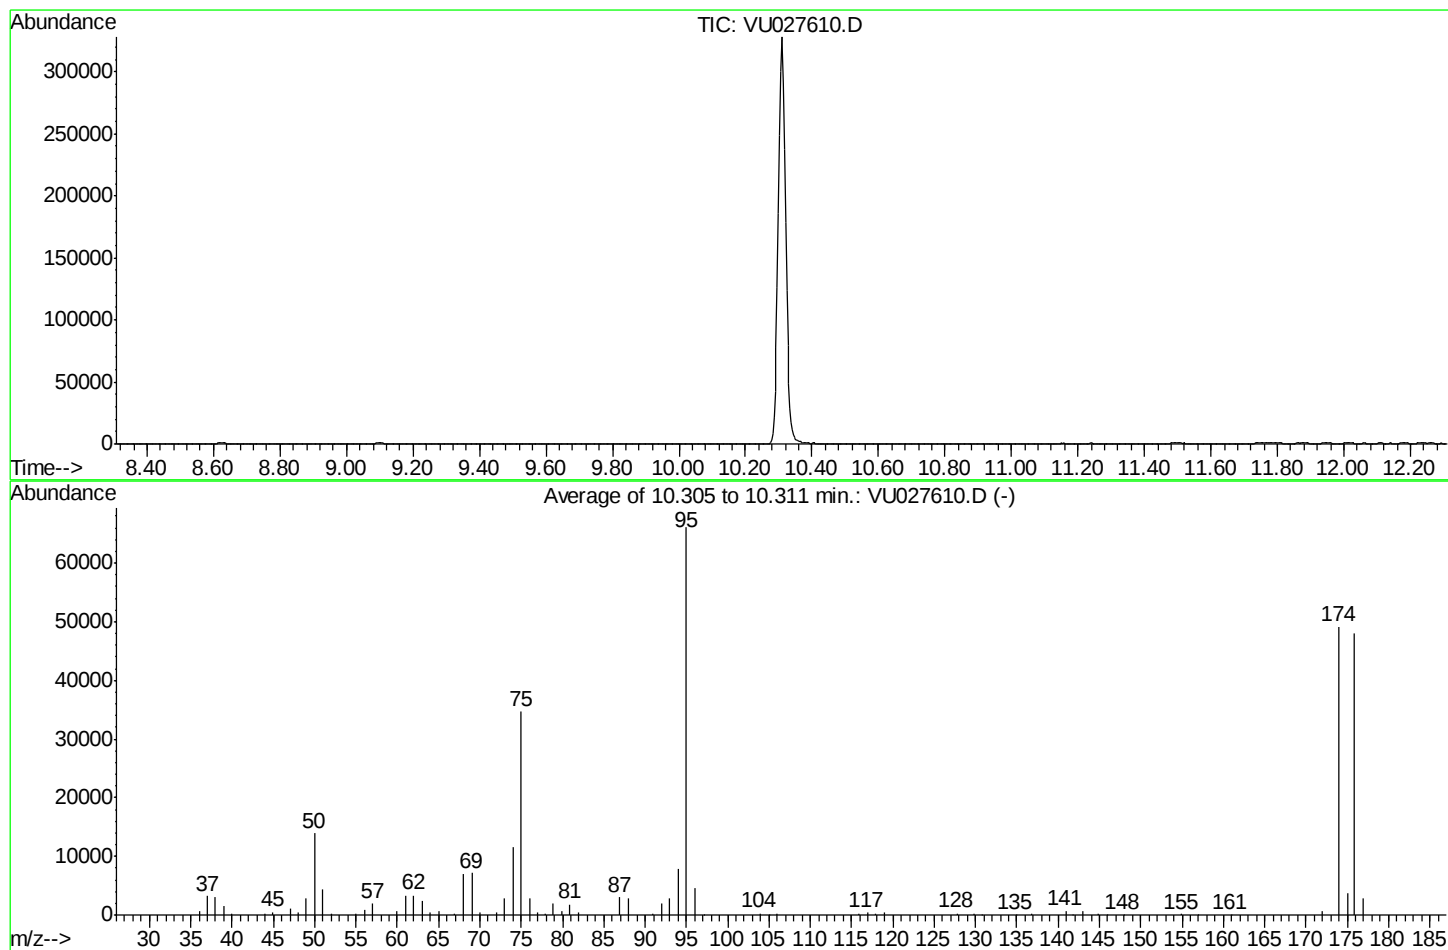

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	13958	PASS
75	95	30	80	52.4	34629	PASS
95	95	100	100	100.0	66090	PASS
96	95	5	9	7.0	4631	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.4	49138	PASS
175	174	5	9	7.7	3760	PASS
176	174	95	101	97.9	48098	PASS
177	176	5	9	6.0	2894	PASS

m/z	Abundance
44.00	342.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.00	609.0
37.10	3255.0
38.00	3150.0
39.00	1509.0
40.00	138.0
44.00	591.0
45.00	535.0
47.10	1142.0
48.00	356.0
49.00	3004.0
50.00	14388.0
51.00	4424.0
52.00	246.0
54.90	135.0
56.00	958.0
57.00	1993.0
60.00	703.0
61.00	3358.0
62.00	3529.0
63.00	2568.0
64.00	370.0
65.00	596.0
66.90	236.0
68.00	7282.0
69.00	7429.0
70.00	500.0
71.90	397.0
73.00	2971.0
74.00	11922.0
75.00	35904.0
76.00	3037.0
76.90	448.0
77.90	293.0
78.90	1968.0
80.00	572.0
80.90	1916.0
82.00	359.0
86.90	3130.0
87.90	2855.0
90.90	234.0
92.00	2139.0
93.00	2968.0
94.00	8251.0
95.00	68224.0
96.00	4818.0
97.10	115.0
103.90	287.0
105.00	103.0
105.90	254.0
115.80	198.0
116.90	451.0
118.00	256.0
118.90	347.0
127.80	255.0
129.80	219.0
130.80	126.0
134.90	104.0
136.80	155.0
140.90	701.0
141.70	100.0
143.00	685.0
144.90	155.0
147.90	112.0
155.00	172.0
156.90	121.0
160.90	104.0
171.90	610.0
174.00	50592.0
175.00	3833.0
175.90	49744.0
177.00	2961.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.00	586.0
37.00	3207.0
38.00	3114.0
39.00	1403.0
39.90	138.0
44.00	607.0
45.00	537.0
47.10	1031.0
48.00	341.0
49.00	2843.0
50.00	13777.0
51.00	4068.0
52.00	239.0
55.00	155.0
56.00	913.0
57.10	1843.0
60.00	652.0
61.00	3120.0
62.00	3163.0
63.00	2494.0
64.00	352.0
65.00	524.0
66.90	219.0
68.00	6614.0
69.00	7033.0
70.00	474.0
72.00	348.0
73.00	2800.0
74.00	10898.0
75.00	32952.0
76.00	2952.0
76.90	435.0
77.90	293.0
78.90	1852.0
80.00	553.0
80.90	1672.0
81.90	345.0
86.90	2814.0
87.90	2702.0
90.90	211.0
92.00	2014.0
93.00	2674.0
94.00	7459.0
95.00	62544.0
96.00	4485.0
97.20	106.0
103.90	273.0
105.90	218.0
115.90	165.0
116.90	380.0
118.00	240.0
118.90	315.0
127.80	227.0
129.80	199.0
136.80	146.0
140.90	621.0
142.90	629.0
144.90	139.0
155.00	135.0
156.90	121.0
171.90	520.0
174.00	45792.0
175.00	3601.0
175.90	44232.0
177.00	2841.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.00	550.0
37.10	3113.0
38.00	2919.0
39.00	1517.0
40.10	114.0
44.00	545.0
44.90	522.0
47.10	1091.0
47.90	369.0
49.00	2866.0
50.00	13710.0
51.00	4334.0
52.00	230.0
55.00	108.0
56.00	934.0
57.00	1988.0
60.00	646.0
61.00	3232.0
62.00	3450.0
63.00	2475.0
63.90	338.0
65.00	578.0
66.90	230.0
68.00	7185.0
69.00	7065.0
70.00	521.0
71.90	406.0
73.00	3022.0
74.00	11663.0
75.00	35032.0
76.00	2760.0
76.90	444.0
78.00	285.0
78.90	1917.0
79.90	553.0
80.90	1932.0
82.00	357.0
87.00	3070.0
88.00	2871.0
90.90	264.0
92.00	2043.0
93.00	2995.0
94.00	8184.0
95.00	67504.0
96.00	4590.0
97.00	112.0
103.90	286.0
105.00	107.0
105.90	273.0
115.80	232.0
116.90	446.0
117.90	215.0
118.90	362.0
127.80	249.0
129.80	218.0
130.80	115.0
134.90	124.0
136.80	136.0
140.90	689.0
142.90	669.0
144.90	171.0
145.90	101.0
147.90	155.0
154.90	192.0
156.90	100.0
171.90	643.0
174.00	51032.0
175.00	3847.0
175.90	50320.0
177.00	2880.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42