

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101219\
 Data File : VU035126.D
 Acq On : 12 Oct 2019 06:55
 Operator : JC/SP
 Sample : K5309-13
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 RD-2-001-01

Quant Time: Oct 14 02:11:06 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Oct 14 01:16:14 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	168029	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	177450	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.47	152	67836	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	46266	4.66	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.20%
7) Chloroethane-d5	1.68	69	43687	4.71	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.20%
11) 1,1-Dichloroethene-d2	2.26	63	68624	3.28	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.60%
20) 2-Butanone-d5	4.17	46	146665	50.14	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.28%
24) Chloroform-d	4.62	84	88234	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.00%
26) 1,2-Dichloroethane-d4	5.29	65	52199	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.80%
32) Benzene-d6	5.32	84	172148	4.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.80%
36) 1,2-Dichloropropane-d6	6.31	67	60996	4.39	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.80%
41) Toluene-d8	7.55	98	147711	3.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.40%
43) trans-1,3-Dichloropropene-	7.84	79	17346	3.47	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	69.40%
46) 2-Hexanone-d5	8.30	63	104997	44.10	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.20%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	53528	4.57	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.40%
64) 1,2-Dichlorobenzene-d4	11.84	152	54226	4.74	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.80%


Target Compounds					Ovalue
13) Acetone	2.31	43	3484	1.454 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU101219\
Data File : VU035126.D
Acq On : 12 Oct 2019 06:55
Operator : JC/SP
Sample : K5309-13
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
RD-2-001-01

Quant Time: Oct 14 02:11:06 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Oct 14 01:16:14 2019
Response via : Initial Calibration

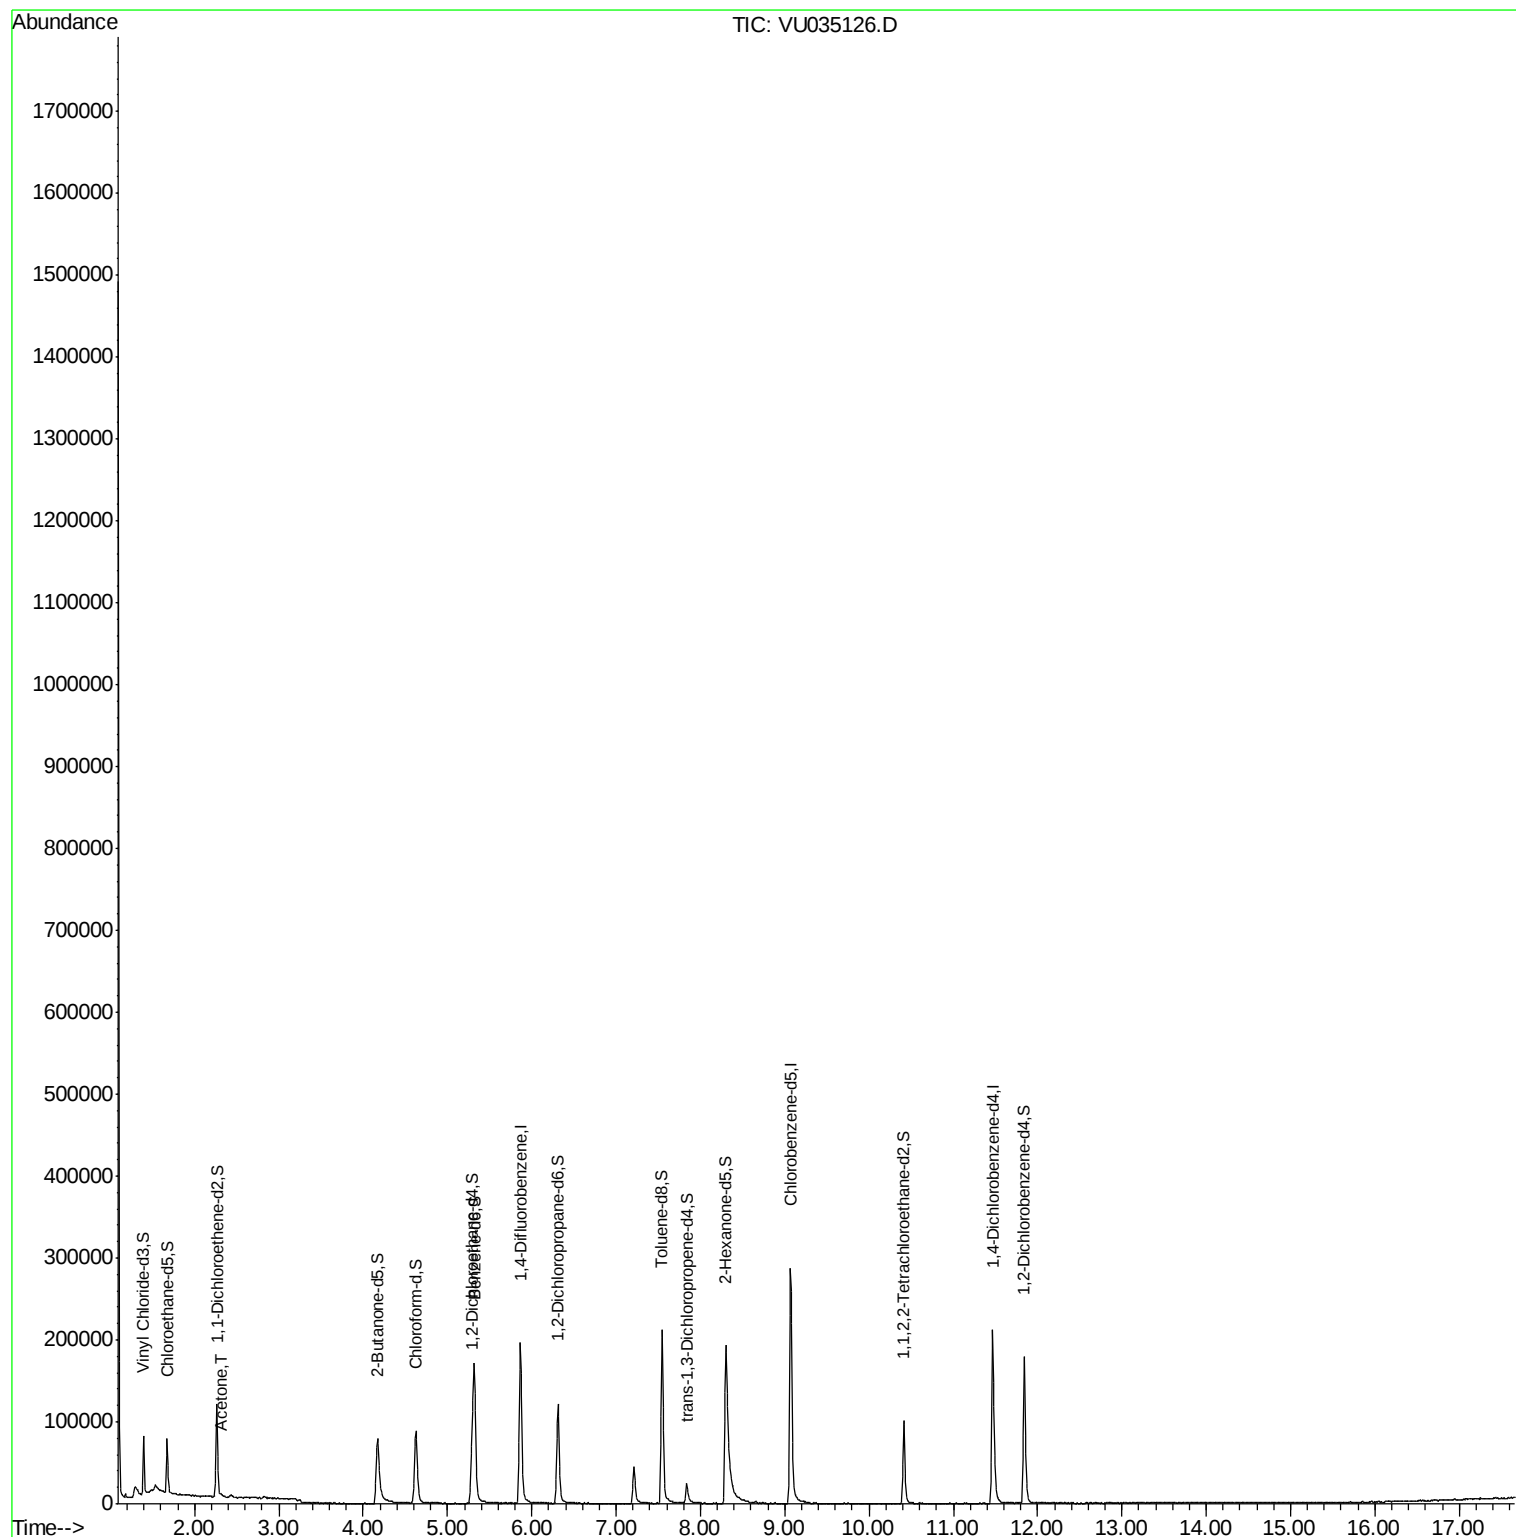

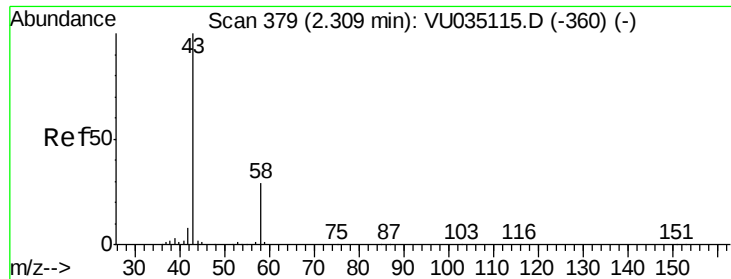

#13

Acetone

Concen: 1.454 ug/L

RT: 2.31 min Scan# 379

Delta R.T. 0.00 min

Lab File: VU035126.D

Acq: 12 Oct 2019 06:55

Instrument :

MSVOA_U

ClientSampleId :

RD-2-001-01

Tot Ion: 43 Resp: 3484

Ion Ratio Lower Upper

43 100

58 31.6 0.0 66.6

