

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U101219\
 Data File : VU035134.D
 Acq On : 12 Oct 2019 10:10
 Operator : JC/SP
 Sample : K5310-19
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 OU2-MW-1-001-01

Quant Time: Oct 14 03:47:10 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Oct 14 01:16:14 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.87	114	167190	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	174283	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.47	152	65488	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	52216	5.28	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	105.60%
7) Chloroethane-d5	1.68	69	49825	5.40	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.00%
11) 1,1-Dichloroethene-d2	2.26	63	78453	3.76	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.20%
20) 2-Butanone-d5	4.17	46	149966	51.53	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.06%
24) Chloroform-d	4.63	84	95321	5.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.20%
26) 1,2-Dichloroethane-d4	5.29	65	56659	5.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.40%
32) Benzene-d6	5.32	84	196724	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.20%
36) 1,2-Dichloropropane-d6	6.31	67	70954	5.19	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.80%
41) Toluene-d8	7.55	98	169475	4.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.80%
43) trans-1,3-Dichloropropene-	7.84	79	19428	3.95	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.00%
46) 2-Hexanone-d5	8.30	63	110628	47.31	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.62%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	56840	4.94	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.80%
64) 1,2-Dichlorobenzene-d4	11.84	152	59739	5.41	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.20%

Target Compounds


					Ovalue
13) Acetone	2.31	43	3686	1.546 ug/L	94
22) cis-1,2-Dichloroethene	4.20	96	6138	0.479 ug/L	99
47) Tetrachloroethene	8.21	164	8911	0.813 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101219\
Data File : VU035134.D
Acq On : 12 Oct 2019 10:10
Operator : JC/SP
Sample : K5310-19
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 61 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
OU2-MW-1-001-01

Quant Time: Oct 14 03:47:10 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Oct 14 01:16:14 2019
Response via : Initial Calibration

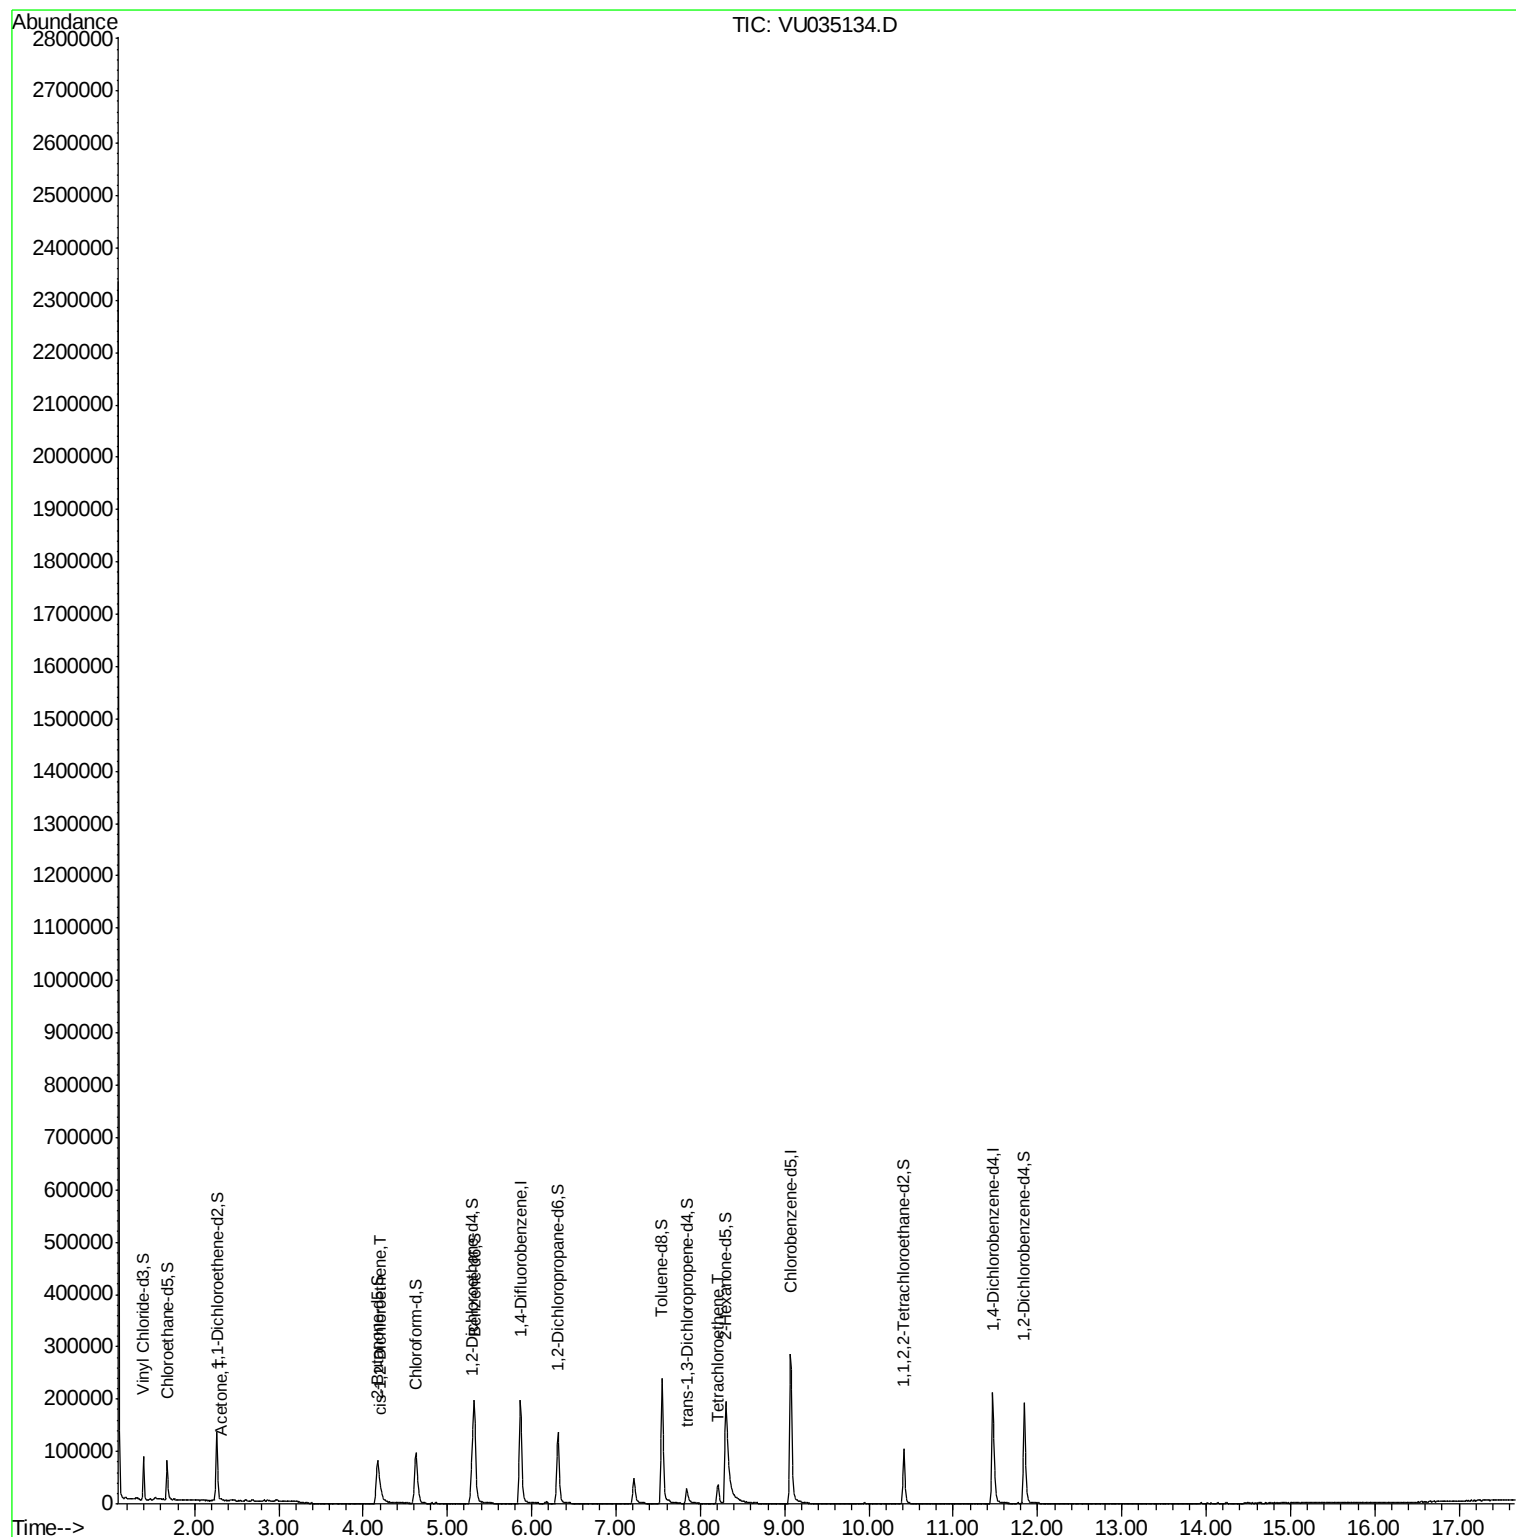

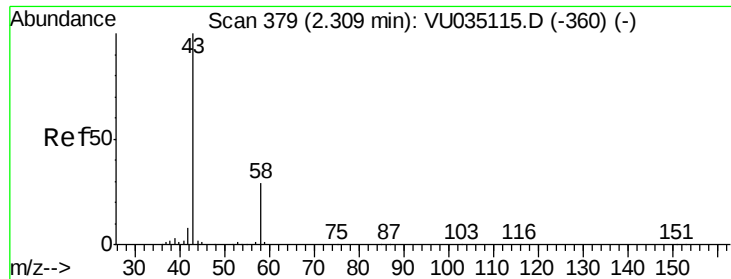

#13

Acetone

Concen: 1.546 ug/L

RT: 2.31 min Scan# 380

Delta R.T. 0.00 min

Lab File: VU035134.D

Acq: 12 Oct 2019 10:10

Instrument :

MSVOA_U

ClientSampleId :


OU2-MW-1-001-01

Tot Ion: 43 Resp: 3686

Ion Ratio Lower Upper




43 100

58 30.1 0.0 66.6

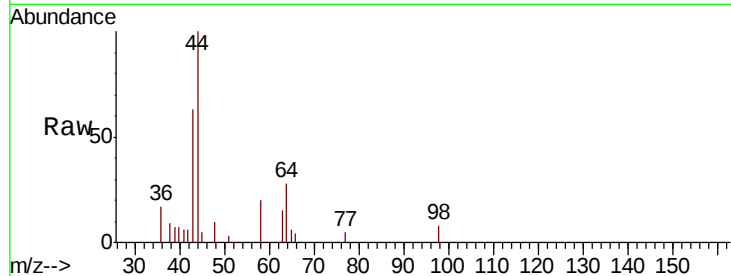

Abundance Ion 43.05 (42.75 to 43.75): VU035115.D (-360) (-)

Ion 58.05 (57.75 to 58.75): VU035115.D (-360) (-)

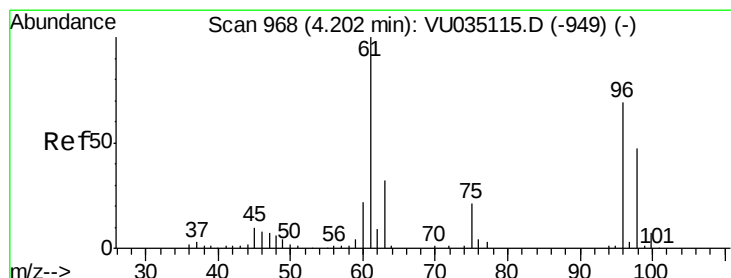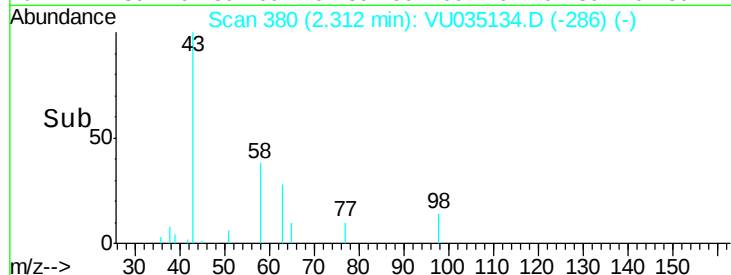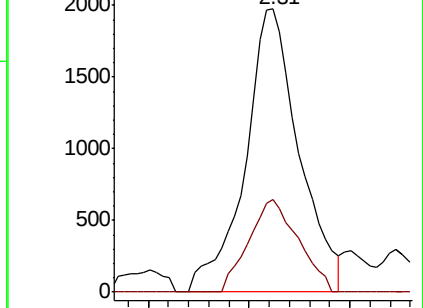

#22

cis-1,2-Dichloroethene

Concen: 0.479 ug/L

RT: 4.20 min Scan# 968

Delta R.T. 0.00 min

Lab File: VU035134.D

Acq: 12 Oct 2019 10:10


Tgt Ion: 96 Resp: 6138

Ion Ratio Lower Upper

96 100

61 128.3 89.2 165.6



68 0.0 0.0 0.0

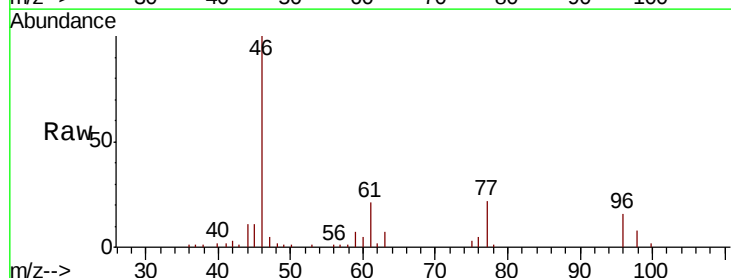


Abundance Ion 96.00 (95.70 to 96.70): VU035115.D (-949) (-)

Ion 61.05 (60.75 to 61.75): VU035115.D (-949) (-)

Ion 68.15 (67.85 to 68.85): VU035115.D (-949) (-)

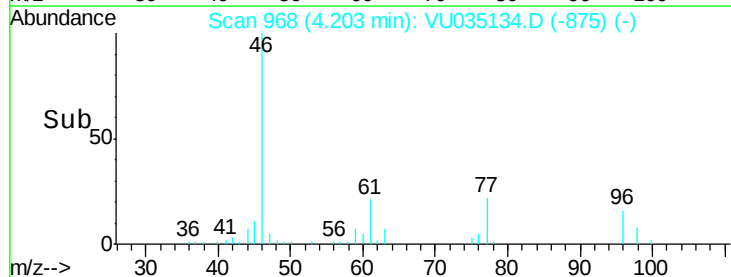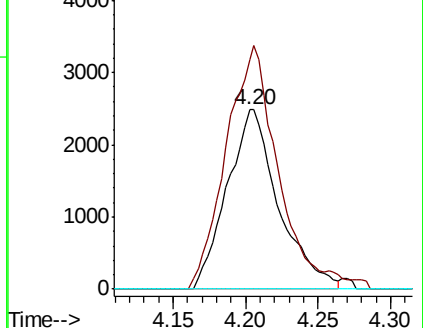

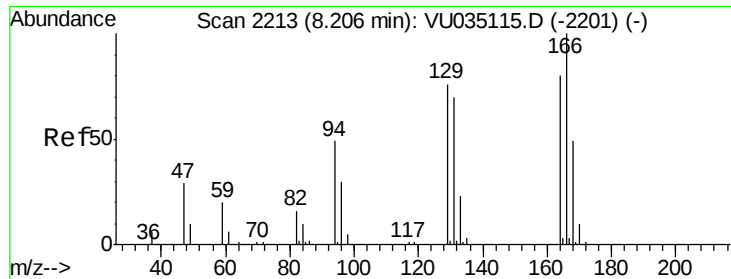

#47

Tetrachloroethene

Concen: 0.813 ug/L

RT: 8.21 min Scan# 2214

Delta R.T. 0.00 min

Lab File: VU035134.D


Acq: 12 Oct 2019 10:10

Instrument :

MSVOA_U

ClientSampleId :

OU2-MW-1-001-01

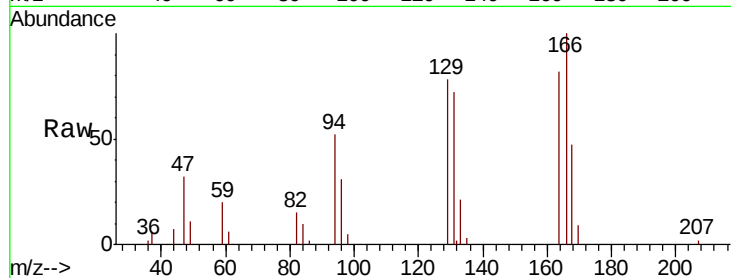

Tot Ion:164 Resp: 8911

Ion Ratio Lower Upper

164 100

129 95.0 68.5 127.1

131 87.5 67.3 124.9

166 121.6 93.1 172.9

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

