


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101219\
Data File : VU035076.D
Acq On : 11 Oct 2019 08:26
Operator : JC/SP
Sample : BFB18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB18

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Oct 15 06:32:18 2019

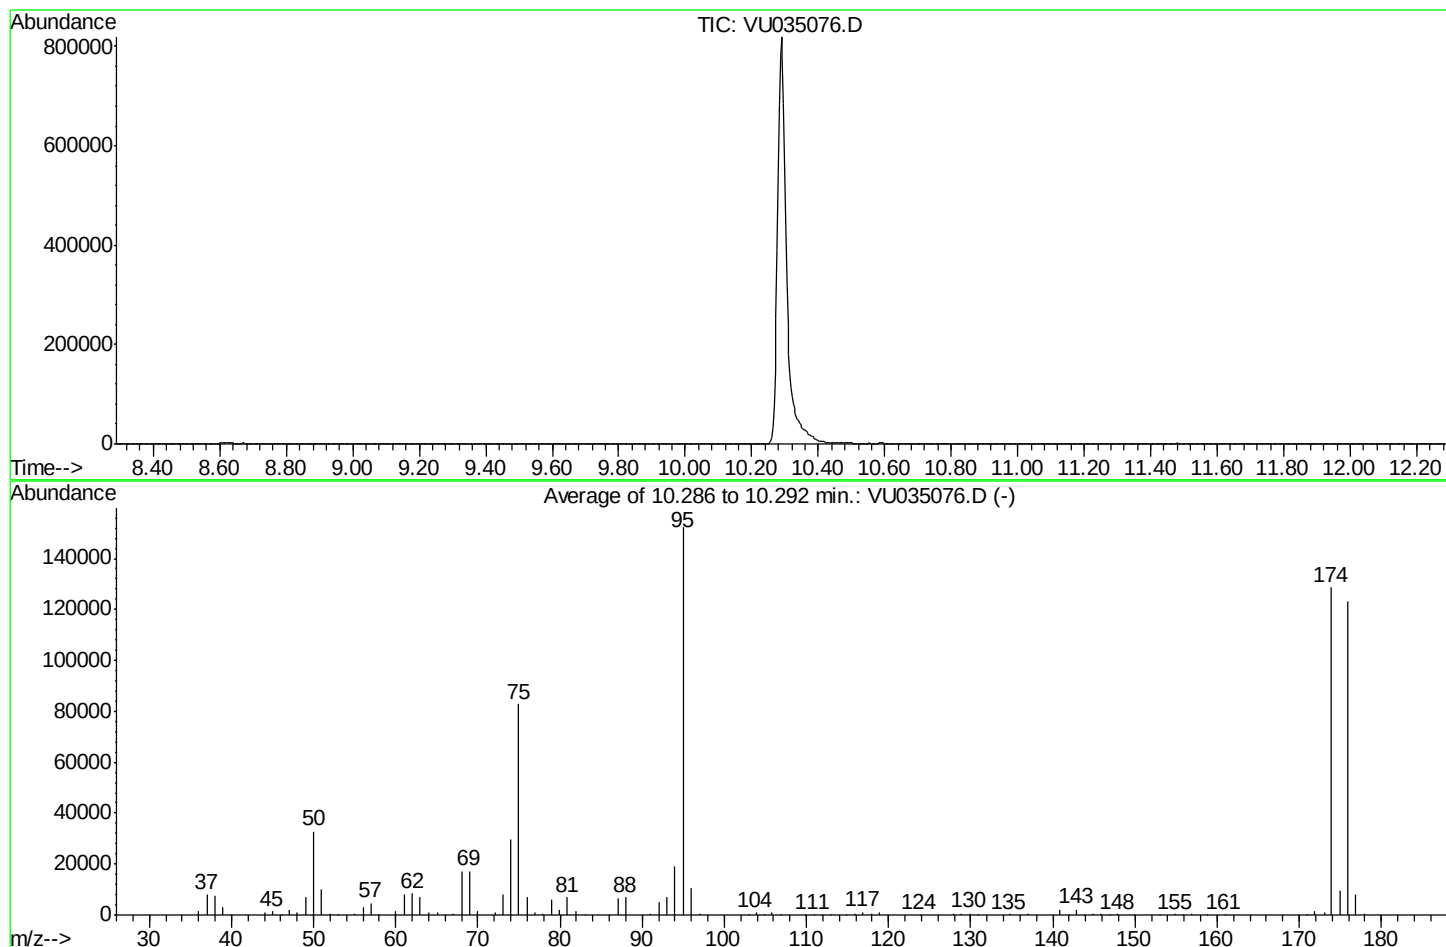

AutoFind: Scans 2860, 2861, 2862; Background Corrected with Scan 2847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	32904	PASS
75	95	30	80	54.4	82792	PASS
95	95	100	100	100.0	152234	PASS
96	95	5	9	6.8	10399	PASS
173	174	0.00	2	1.0	1242	PASS
174	95	50	120	84.4	128522	PASS
175	174	5	9	7.5	9702	PASS
176	174	95	101	96.0	123378	PASS
177	176	5	9	6.4	7917	PASS

Scan 2847 (10.244 min): VU035076.D
BFB18

m/z	Abundance
39.90	191.0
44.00	475.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18

m/z	Abundance
36.00	1381.0
37.00	8260.0
38.00	7561.0
39.00	3233.0
40.00	290.0
44.00	1424.0
45.00	1523.0
46.10	214.0
47.00	2062.0
48.00	1044.0
49.00	7241.0
50.00	32784.0
51.00	9909.0
52.00	426.0
52.90	171.0
55.00	422.0
56.00	3000.0
57.00	4620.0
57.90	203.0
60.00	1573.0
61.00	8374.0
62.00	8392.0
63.00	7115.0
64.00	1031.0
65.00	1219.0
66.10	175.0
66.90	370.0
68.00	16784.0
69.00	17288.0
70.00	1445.0
72.10	1001.0
73.00	8131.0
74.00	29736.0
75.00	82312.0
76.00	6789.0
76.90	979.0
78.00	771.0
78.90	6368.0
79.90	1879.0
80.90	6778.0
81.90	1511.0
82.90	252.0
86.00	252.0
87.00	6637.0
88.00	6611.0
90.90	619.0
92.00	4921.0
93.00	7270.0
94.00	19488.0
95.00	151744.0
96.00	10632.0
97.00	306.0
102.90	131.0
103.90	812.0
104.80	211.0
105.80	768.0
106.90	170.0
109.90	137.0
110.80	171.0
111.80	132.0
112.90	166.0
114.90	157.0
115.90	629.0
116.90	1167.0
117.90	615.0
118.90	997.0
123.80	159.0
127.90	486.0
128.90	322.0
129.90	508.0
130.80	249.0
134.80	270.0
136.90	225.0
140.90	1845.0
141.90	257.0
142.90	2342.0
143.80	120.0
144.90	460.0
145.90	327.0
146.90	129.0
147.90	371.0
149.90	129.0
153.00	105.0
154.90	474.0
155.90	141.0
156.90	270.0
158.80	157.0
160.90	140.0
170.80	215.0
171.90	1505.0
173.90	125040.0
175.00	9219.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18

175.90	118568.0
176.90	7663.0
177.90	237.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18

m/z	Abundance
36.00	1553.0
37.00	8095.0
38.00	7684.0
39.00	3239.0
39.90	311.0
44.00	1520.0
45.00	1475.0
46.00	216.0
47.00	2128.0
48.00	1035.0
49.00	7356.0
50.00	34032.0
51.00	10331.0
52.00	427.0
53.00	168.0
55.00	440.0
56.00	3093.0
57.00	4729.0
57.90	205.0
60.00	1755.0
61.00	8437.0
62.00	8615.0
63.00	7211.0
64.00	1077.0
65.00	1281.0
66.00	126.0
66.90	426.0
68.00	17592.0
69.00	17784.0
70.00	1557.0
72.10	1086.0
73.00	8532.0
74.00	30736.0
75.00	85416.0
76.00	7028.0
76.90	1077.0
78.00	766.0
78.90	6398.0
79.90	1815.0
80.90	7223.0
81.90	1534.0
82.90	232.0
86.10	263.0
87.00	6825.0
88.00	7227.0
90.90	628.0
92.00	5096.0
93.00	7488.0
94.00	19688.0
95.00	156800.0
96.00	10681.0
97.00	296.0
102.90	108.0
103.90	932.0
104.80	202.0
105.80	932.0
106.90	171.0
109.80	145.0
110.90	174.0
111.90	141.0
112.90	179.0
114.80	173.0
115.90	670.0
116.90	1310.0
117.90	668.0
118.90	986.0
123.80	182.0
127.90	499.0
128.90	300.0
129.90	536.0
130.80	237.0
134.70	318.0
136.90	305.0
140.90	1889.0
141.80	228.0
142.90	2358.0
143.90	120.0
144.90	421.0
145.90	328.0
146.80	162.0
147.90	409.0
149.90	146.0
153.00	134.0
154.90	516.0
155.80	109.0
156.90	291.0
158.80	208.0
160.90	144.0
170.80	228.0
171.90	1520.0
173.10	1856.0
173.90	132416.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18

175.00	9965.0
175.90	127064.0
176.90	8134.0
177.90	301.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18

m/z	Abundance
36.00	1592.0
37.00	7545.0
38.00	7191.0
39.00	2917.0
40.00	313.0
44.00	1495.0
45.00	1320.0
46.00	212.0
47.00	1893.0
48.00	921.0
49.00	6665.0
50.00	31896.0
51.00	9903.0
52.00	411.0
53.00	136.0
55.00	472.0
56.00	2925.0
57.00	4442.0
58.00	192.0
60.00	1717.0
61.00	8098.0
62.00	8105.0
63.00	6542.0
64.00	967.0
65.10	1239.0
66.90	437.0
68.00	16544.0
69.00	16944.0
70.00	1479.0
72.10	956.0
73.00	8141.0
74.00	28616.0
75.00	80648.0
76.00	6636.0
77.00	1009.0
77.90	733.0
78.90	5980.0
79.90	1636.0
80.90	6822.0
81.90	1369.0
83.00	172.0
86.10	290.0
87.00	6556.0
88.00	7067.0
90.90	657.0
92.00	4753.0
93.00	7045.0
94.00	18312.0
95.00	148160.0
96.00	9885.0
97.00	293.0
103.90	894.0
104.80	198.0
105.90	892.0
106.80	157.0
109.80	136.0
110.90	167.0
112.00	170.0
112.90	189.0
114.90	189.0
115.90	699.0
116.90	1303.0
117.90	642.0
118.90	928.0
123.80	167.0
127.80	466.0
128.90	268.0
129.90	505.0
130.90	236.0
134.70	338.0
136.90	348.0
140.90	1807.0
141.80	197.0
142.90	2138.0
143.90	101.0
144.90	396.0
145.90	253.0
146.80	126.0
147.90	416.0
149.90	146.0
152.90	148.0
154.90	456.0
156.90	281.0
158.80	221.0
160.90	161.0
170.90	227.0
171.90	1512.0
173.10	1872.0
173.90	128112.0
175.00	9924.0
175.90	124504.0
176.90	7955.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18

177.90

283.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18