

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101221\
 Data File : VU045285.D
 Acq On : 12 Oct 2021 12:04
 Operator : SY/MD
 Sample : VU1012WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK029

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

Signal : TIC: VU045285.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.469	34	40	52	rVB	10830	19444	1.48%	0.199%
2	1.601	73	81	92	rBV	185967	200129	15.26%	2.047%
3	1.883	161	169	184	rVB	135077	183281	13.98%	1.875%
4	2.559	366	379	406	rBV	257974	436254	33.27%	4.462%
5	2.694	418	421	424	rBV	446	360	0.03%	0.004%
6	2.787	441	450	459	rVB	1274	2289	0.17%	0.023%
7	2.957	494	503	515	rVB2	1287	1964	0.15%	0.020%
8	3.041	522	529	538	rVV4	1555	2666	0.20%	0.027%
9	3.125	551	555	558	rBV	201	164	0.01%	0.002%
10	3.192	571	576	578	rBV3	289	272	0.02%	0.003%
11	3.224	583	586	590	rVV2	178	168	0.01%	0.002%
12	3.346	621	624	631	rVB3	503	534	0.04%	0.005%
13	3.382	631	635	637	rBV	166	159	0.01%	0.002%
14	3.465	655	661	664	rBV2	196	261	0.02%	0.003%
15	3.581	694	697	702	rBV2	183	192	0.01%	0.002%
16	4.002	821	828	831	rBV	199	239	0.02%	0.002%
17	4.324	926	928	932	rVB2	257	179	0.01%	0.002%
18	4.359	932	939	942	rBV2	276	429	0.03%	0.004%
19	4.417	953	957	963	rBV2	189	275	0.02%	0.003%
20	4.629	1003	1023	1067	rBV	150524	358356	27.33%	3.666%
21	5.067	1141	1159	1182	rVV	230273	503377	38.39%	5.149%
22	5.295	1222	1230	1238	rVB3	744	1412	0.11%	0.014%
23	5.340	1238	1244	1245	rBV	299	258	0.02%	0.003%
24	5.369	1250	1253	1254	rBV3	284	143	0.01%	0.001%
25	5.523	1297	1301	1305	rBV	195	205	0.02%	0.002%
26	5.623	1328	1332	1338	rBV2	196	177	0.01%	0.002%
27	5.729	1342	1365	1392	rBV2	488687	1311073	100.00%	13.411%
28	6.038	1457	1461	1463	rBV2	460	279	0.02%	0.003%
29	6.121	1482	1487	1488	rBV2	225	191	0.01%	0.002%
30	6.253	1513	1528	1545	rBV	341990	631639	48.18%	6.461%
31	6.359	1557	1561	1565	rBV2	219	278	0.02%	0.003%
32	6.411	1572	1577	1581	rBV2	151	209	0.02%	0.002%
33	6.491	1600	1602	1605	rBV2	303	208	0.02%	0.002%
34	6.533	1605	1615	1628	rVB5	3814	7578	0.58%	0.078%
35	6.694	1650	1665	1685	rBV	312008	599593	45.73%	6.133%
36	6.800	1695	1698	1699	rBV	321	212	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101221\
 Data File : VU045285.D
 Acq On : 12 Oct 2021 12:04
 Operator : SY/MD
 Sample : VU1012WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK029

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	7.047	1768	1775	1778	rBV3	483	677	0.05%	0.007%
38	7.086	1784	1787	1790	rBV	224	180	0.01%	0.002%
39	7.185	1807	1818	1827	rVB5	1937	3259	0.25%	0.033%
40	7.314	1854	1858	1861	rBV	240	198	0.02%	0.002%
41	7.337	1861	1865	1867	rBV2	154	135	0.01%	0.001%
42	7.411	1885	1888	1892	rBV	157	155	0.01%	0.002%
43	7.568	1924	1937	1956	rBV	175256	300199	22.90%	3.071%
44	7.690	1969	1975	1984	rVB3	1000	1506	0.11%	0.015%
45	7.800	1998	2009	2018	rBV3	1197	2028	0.15%	0.021%
46	7.899	2025	2040	2056	rBV	587327	1008000	76.88%	10.311%
47	7.973	2056	2063	2073	rVB	8482	14300	1.09%	0.146%
48	8.182	2116	2128	2144	rBV	123589	202043	15.41%	2.067%
49	8.372	2184	2187	2190	rVB3	249	171	0.01%	0.002%
50	8.523	2231	2234	2237	rVB2	192	141	0.01%	0.001%
51	8.549	2237	2242	2243	rBV	168	136	0.01%	0.001%
52	8.558	2243	2245	2249	rVB2	273	194	0.01%	0.002%
53	8.639	2256	2270	2304	rBV	443789	793787	60.54%	8.120%
54	8.832	2327	2330	2339	rVB2	331	366	0.03%	0.004%
55	9.012	2384	2386	2391	rBV	190	208	0.02%	0.002%
56	9.083	2405	2408	2414	rBV2	229	324	0.02%	0.003%
57	9.282	2466	2470	2472	rBV	221	224	0.02%	0.002%
58	9.420	2498	2513	2547	rBV	490743	800603	61.06%	8.189%
59	9.539	2547	2550	2554	rVB2	178	176	0.01%	0.002%
60	9.571	2554	2560	2567	rBV4	755	1062	0.08%	0.011%
61	9.639	2578	2581	2585	rBV	201	210	0.02%	0.002%
62	9.693	2593	2598	2607	rVB2	1198	1651	0.13%	0.017%
63	9.812	2627	2635	2640	rBV2	210	422	0.03%	0.004%
64	9.893	2657	2660	2663	rVB	265	198	0.02%	0.002%
65	9.980	2684	2687	2689	rBV2	207	181	0.01%	0.002%
66	10.108	2720	2727	2730	rBV5	747	986	0.08%	0.010%
67	10.192	2746	2753	2754	rBV	183	199	0.02%	0.002%
68	10.465	2835	2838	2841	rBV2	259	195	0.01%	0.002%
69	10.494	2844	2847	2851	rVB3	492	350	0.03%	0.004%
70	10.674	2894	2903	2912	rVB2	3333	4853	0.37%	0.050%
71	10.761	2916	2930	2947	rBV	453964	725774	55.36%	7.424%
72	10.832	2950	2952	2957	rVB2	726	412	0.03%	0.004%
73	10.899	2970	2973	2976	rVB3	230	162	0.01%	0.002%
74	11.089	3027	3032	3035	rBV4	616	641	0.05%	0.007%
75	11.150	3048	3051	3056	rVB3	371	259	0.02%	0.003%
76	11.298	3095	3097	3101	rVB	249	143	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101221\
 Data File : VU045285.D
 Acq On : 12 Oct 2021 12:04
 Operator : SY/MD
 Sample : VU1012WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK029

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.320	3101	3104	3106	rBV2	250	181	0.01%	0.002%
78	11.462	3140	3148	3160	rVB6	2581	4862	0.37%	0.050%
79	11.700	3213	3222	3229	rBV5	1668	2316	0.18%	0.024%
80	11.748	3231	3237	3245	rVV3	1397	1738	0.13%	0.018%
81	11.816	3245	3258	3286	rVV	457885	719207	54.86%	7.357%
82	11.941	3293	3297	3298	rBV	872	607	0.05%	0.006%
83	11.976	3303	3308	3315	rVB5	2237	3086	0.24%	0.032%
84	12.053	3329	3332	3334	rBV2	207	165	0.01%	0.002%
85	12.124	3351	3354	3361	rBV3	228	205	0.02%	0.002%
86	12.195	3361	3376	3399	rBV	530987	875624	66.79%	8.957%
87	12.333	3417	3419	3424	rVB2	707	594	0.05%	0.006%
88	12.391	3432	3437	3439	rBV2	484	424	0.03%	0.004%
89	12.635	3511	3513	3514	rBV	313	148	0.01%	0.002%
90	12.745	3543	3547	3552	rBV2	311	377	0.03%	0.004%
91	12.983	3618	3621	3624	rBV	192	172	0.01%	0.002%
92	13.005	3624	3628	3632	rVB3	629	598	0.05%	0.006%
93	13.188	3681	3685	3690	rBV2	275	349	0.03%	0.004%
94	13.227	3690	3697	3704	rBV2	1754	2507	0.19%	0.026%
95	13.809	3873	3878	3880	rBV2	216	221	0.02%	0.002%
96	13.844	3882	3889	3903	rVB3	3761	5551	0.42%	0.057%
97	14.092	3957	3966	3983	rVB	11268	18616	1.42%	0.190%
98	14.336	4034	4042	4051	rVB3	4748	7021	0.54%	0.072%
99	14.394	4057	4060	4068	rBV3	298	285	0.02%	0.003%
100	14.950	4231	4233	4237	rBV3	313	231	0.02%	0.002%




Sum of corrected areas: 9776240

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101221\
Data File : VU045285.D
Acq On : 12 Oct 2021 12:04
Operator : SY/MD
Sample : VU1012WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK029

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

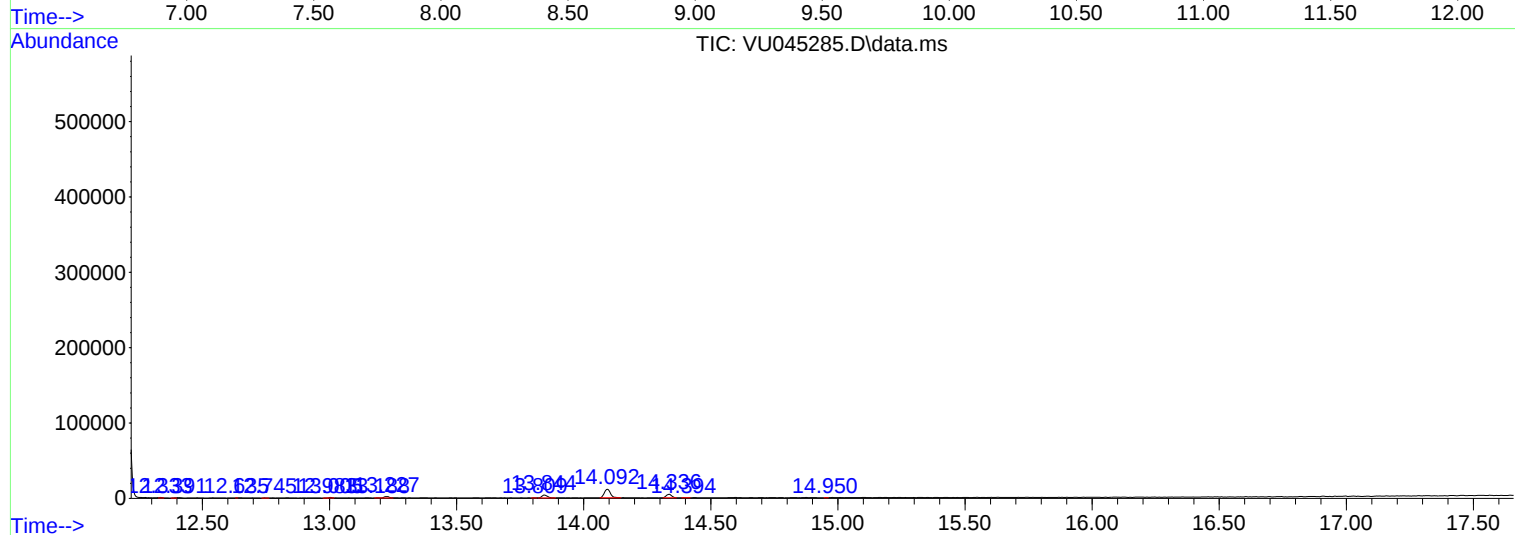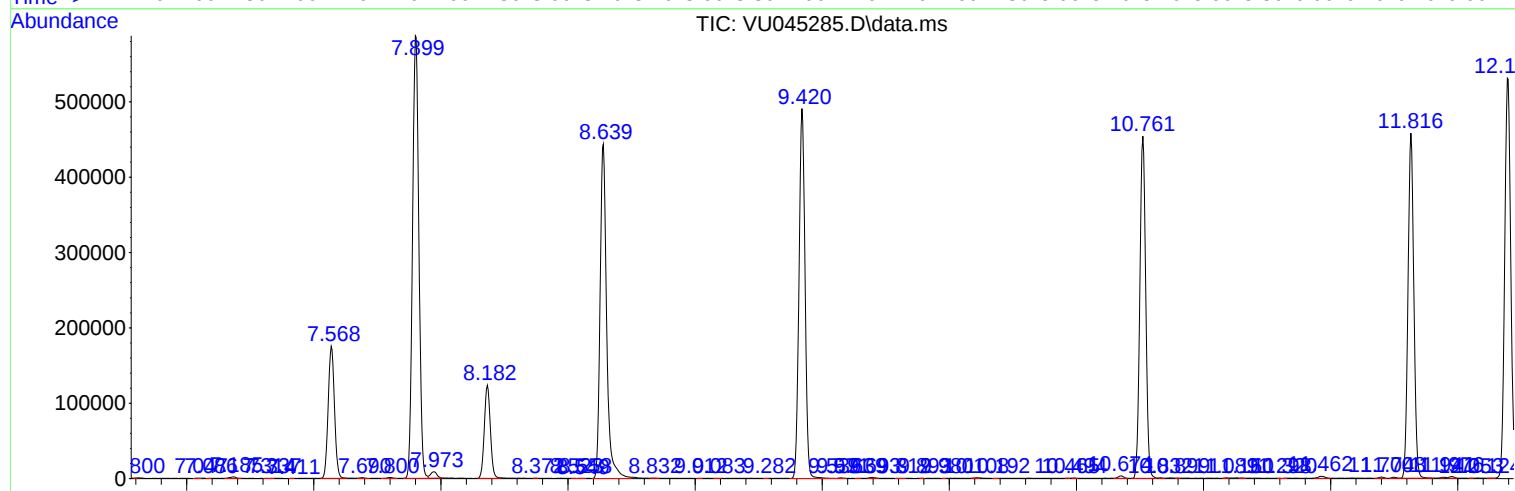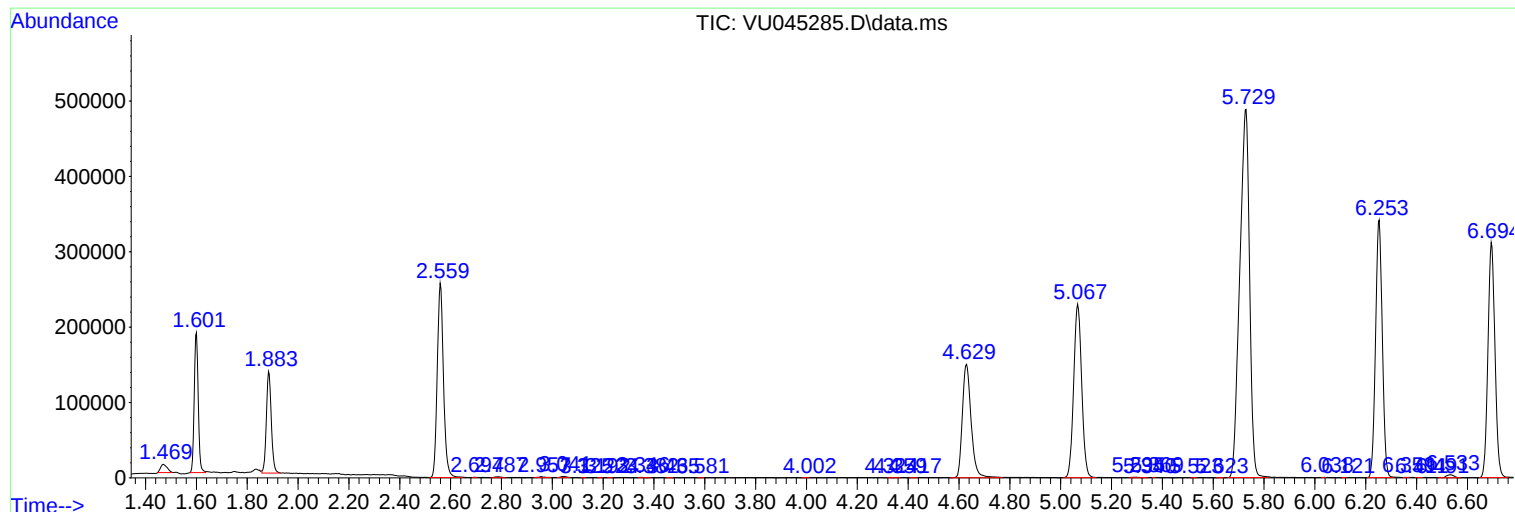

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101221\
Data File : VU045285.D
Acq On : 12 Oct 2021 12:04
Operator : SY/MD
Sample : VU1012WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK029

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101221\
Data File : VU045285.D
Acq On : 12 Oct 2021 12:04
Operator : SY/MD
Sample : VU1012WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK029

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
