
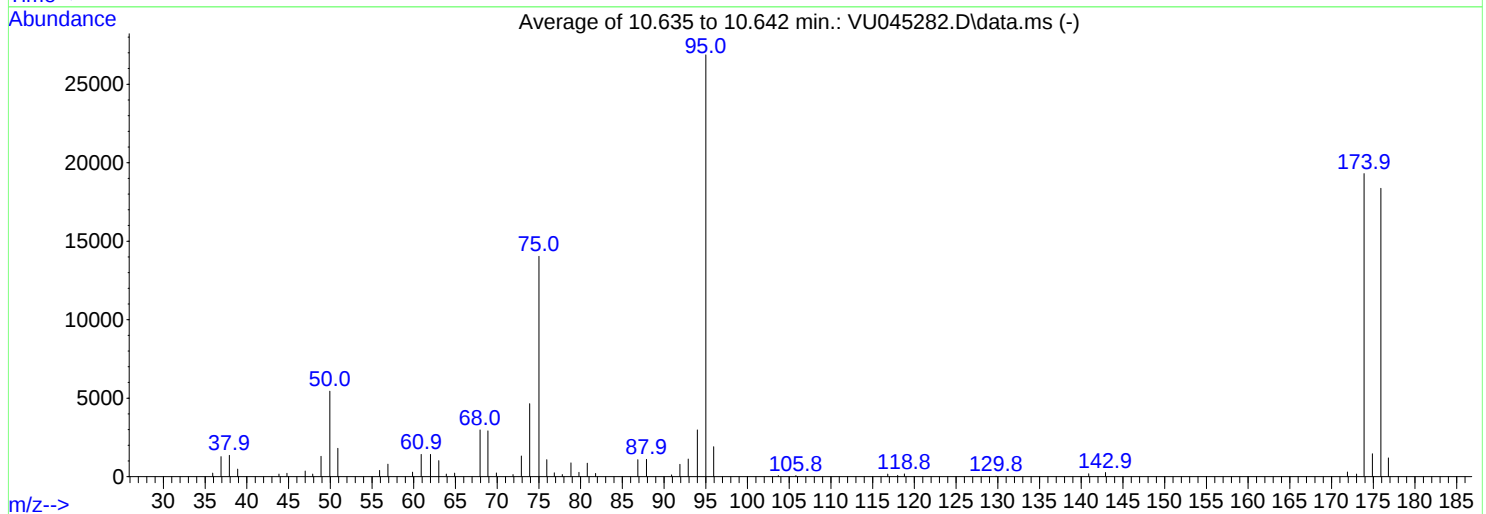


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101221\
 Data File : VU045282.D
 Acq On : 12 Oct 2021 09:37
 Operator : SY/MD
 Sample : BFB012
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB012

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis
 Last Update : Wed Oct 13 02:48:52 2021

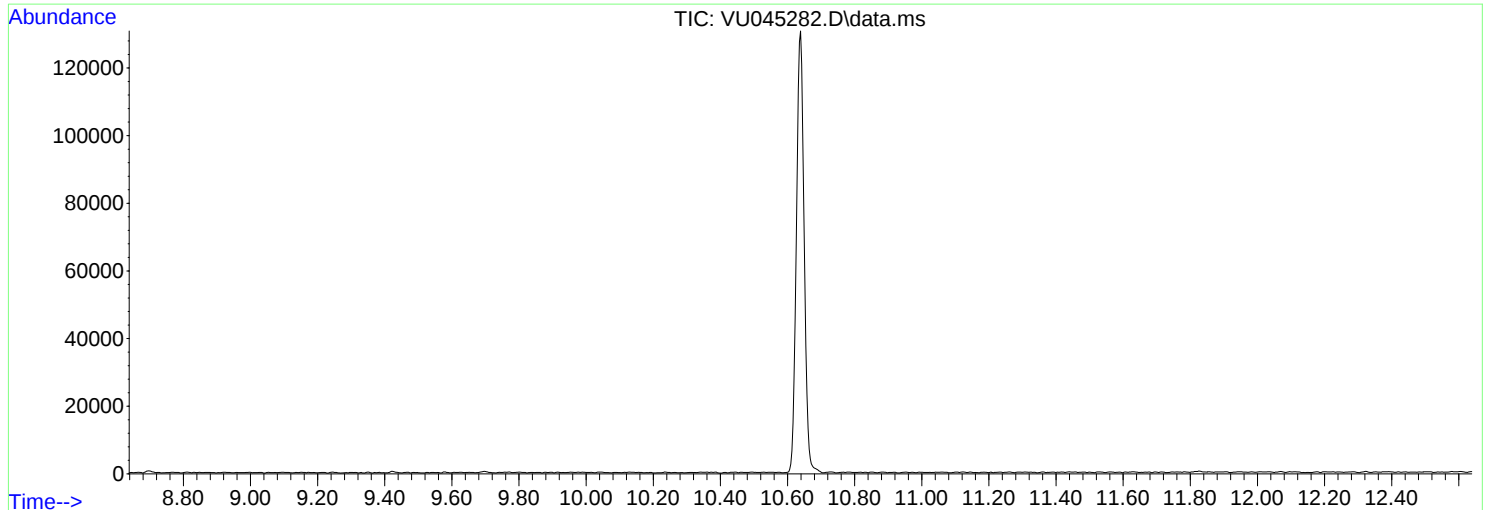

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	5448	PASS
75	95	30	80	52.2	14040	PASS
95	95	100	100	100.0	26872	PASS
96	95	5	9	7.1	1906	PASS
173	174	0.00	2	0.8	161	PASS
174	95	50	120	71.9	19309	PASS
175	174	5	9	7.5	1454	PASS
176	174	95	101	95.1	18371	PASS
177	176	5	9	6.5	1192	PASS

m/z	Abundance
35.90	201.0
36.90	1198.0
37.90	1379.0
38.90	438.0
39.90	116.0
43.80	482.0
44.80	182.0
47.00	340.0
47.90	180.0
48.90	1234.0
50.00	5069.0
50.90	1644.0
55.90	332.0
56.90	807.0
59.80	244.0
60.90	1365.0
62.00	1294.0
63.00	942.0
63.90	168.0
64.90	204.0
67.90	2850.0
68.90	2797.0
69.90	206.0
71.90	119.0
72.90	1226.0
73.90	4318.0
75.00	13197.0
76.00	1028.0
76.90	191.0
77.80	145.0
78.90	861.0
79.80	252.0
80.80	846.0
81.80	190.0
86.90	1030.0
87.90	1050.0
90.90	103.0
91.90	755.0
92.90	1070.0
94.00	2831.0
95.00	25840.0
96.00	1798.0
105.80	100.0
116.80	141.0
118.80	129.0
140.90	139.0
142.90	262.0
171.90	273.0
173.00	236.0
173.90	18728.0
174.90	1388.0
175.90	17928.0
176.80	1258.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012

Scan 2879 (10.597 min): VU045282.D\data.ms
BFB012

m/z	Abundance
39.80	113.0
43.90	301.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012

m/z	Abundance
35.90	242.0
36.90	1315.0
37.90	1270.0
38.90	503.0
43.90	439.0
44.80	247.0
47.00	368.0
47.90	154.0
48.90	1303.0
49.90	5637.0
50.90	1883.0
55.90	464.0
56.90	754.0
59.90	327.0
60.90	1404.0
62.00	1498.0
63.00	1061.0
63.90	163.0
64.90	250.0
68.00	2959.0
68.90	2927.0
69.90	251.0
71.90	149.0
72.90	1344.0
73.90	4842.0
75.00	14437.0
75.90	1095.0
76.80	268.0
77.80	114.0
78.80	885.0
79.80	290.0
80.80	819.0
81.80	219.0
86.80	1106.0
87.90	1151.0
90.90	119.0
91.90	797.0
92.90	1123.0
94.00	3037.0
95.00	27000.0
95.90	1933.0
103.70	104.0
116.80	184.0
118.00	131.0
118.80	206.0
140.90	206.0
142.90	248.0
171.90	305.0
173.90	19280.0
174.90	1465.0
175.90	18264.0
176.80	1079.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012

m/z	Abundance
35.90	236.0
36.90	1298.0
37.90	1420.0
38.90	483.0
43.80	458.0
44.80	226.0
47.00	376.0
47.90	167.0
48.90	1359.0
49.90	5638.0
50.90	1894.0
55.90	409.0
56.90	811.0
59.90	295.0
60.90	1483.0
62.00	1449.0
63.00	1050.0
63.90	156.0
64.90	232.0
68.00	3113.0
68.90	3036.0
69.90	234.0
71.90	129.0
72.90	1365.0
73.90	4797.0
75.00	14486.0
75.90	1113.0
76.90	267.0
77.80	139.0
78.90	900.0
79.80	282.0
80.80	890.0
81.80	205.0
86.90	1114.0
87.90	1114.0
90.90	114.0
91.90	795.0
92.90	1171.0
94.00	3056.0
95.00	27776.0
96.00	1988.0
103.70	102.0
105.80	111.0
116.80	160.0
118.00	117.0
118.80	173.0
129.80	101.0
140.90	191.0
142.90	282.0
171.90	304.0
173.00	247.0
173.90	19920.0
174.90	1509.0
175.90	18920.0
176.80	1238.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012