

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
 Data File : VU051397.D
 Acq On : 12 Oct 2022 18:33
 Operator : JC/MD
 Sample : N5070-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BS7

Quant Time: Oct 13 01:42:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 13 01:37:29 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	182113	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	203977	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	67943	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	88731	6.040	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 120.800%		
7) Chloroethane-d5	1.909	69	64735	5.129	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 102.600%		
11) 1,1-Dichloroethene-d2	2.562	65	30941	5.328	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 106.600%		
20) 2-Butanone-d5	4.639	46	150914	46.661	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	= 93.320%		
24) Chloroform-d	5.060	84	128649	4.697	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 94.000%		
26) 1,2-Dichloroethane-d4	5.703	65	70709	5.006	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 100.200%		
32) Benzene-d6	5.726	84	240534	4.287	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 85.800%		
36) 1,2-Dichloropropane-d6	6.690	67	85086	4.465	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 89.200%		
41) Toluene-d8	7.896	98	171964	3.425	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 68.600%#		
43) trans-1,3-Dichloroprop...	8.179	79	24439	3.903	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 78.000%		
46) 2-Hexanone-d5	8.636	63	80699	38.243	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 76.480%		
56) 1,1,2,2-Tetrachloroeth...	10.754	84	65499	4.303	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 86.000%		
66) 1,2-Dichlorobenzene-d4	12.192	152	53222	4.507	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 90.200%		
Target Compounds						Qvalue
13) Acetone	2.652	43	6732	2.775	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
Data File : VU051397.D
Acq On : 12 Oct 2022 18:33
Operator : JC/MD
Sample : N5070-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BS7

Quant Time: Oct 13 01:42:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 13 01:37:29 2022
Response via : Initial Calibration

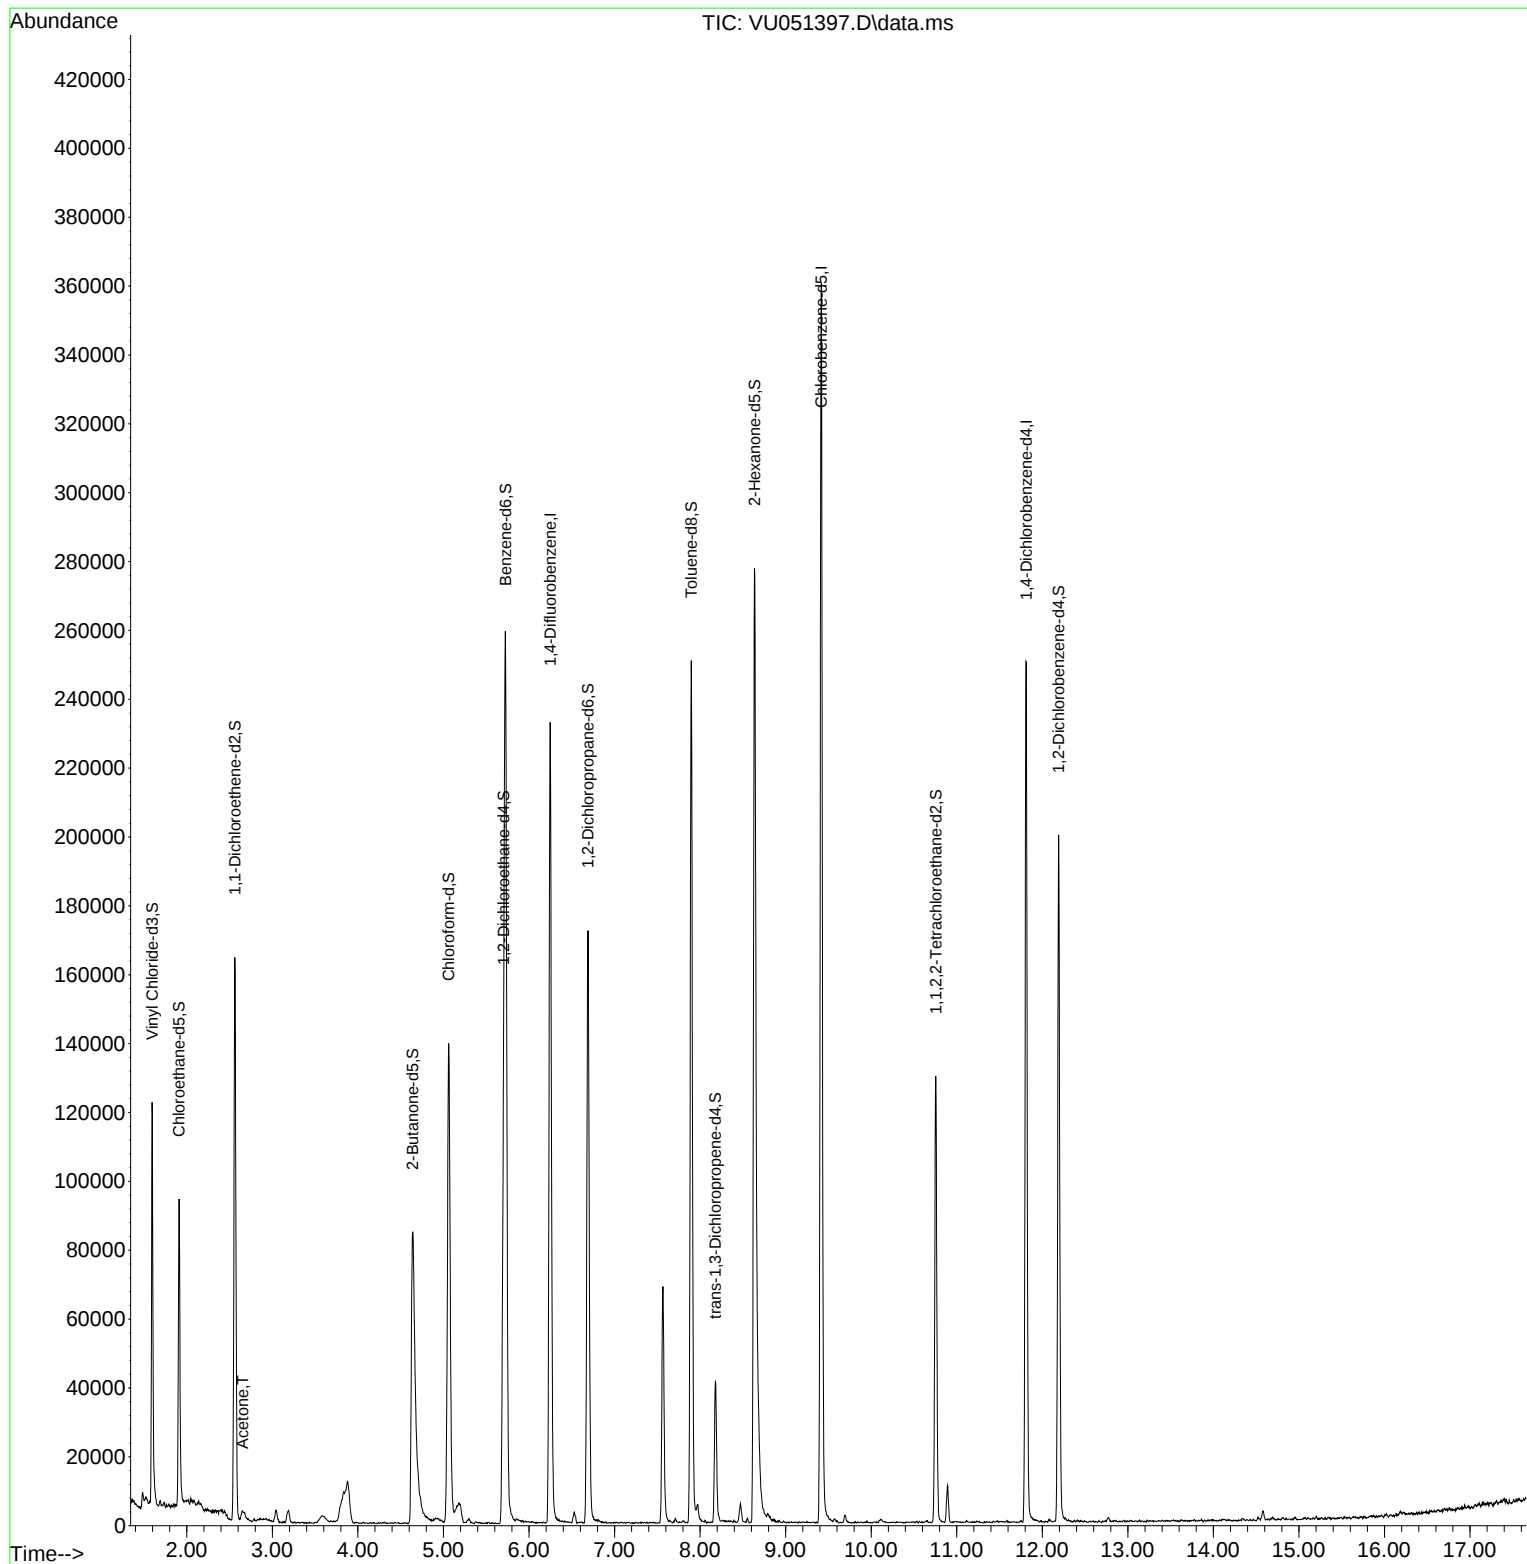

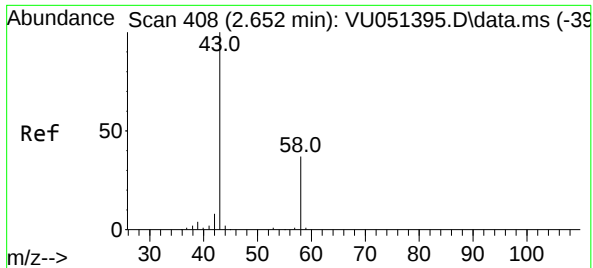

#13
 Acetone
 Concen: 2.775 ug/L
 RT: 2.652 min Scan# 408
 Delta R.T. 0.026 min
 Lab File: VU051397.D
 Acq: 12 Oct 2022 18:33

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BS7

Tgt Ion: 43 Resp: 6732
 Ion Ratio Lower Upper
 43 100
 58 32.1 0.0 68.8

