

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
 Data File : VU051399.D
 Acq On : 12 Oct 2022 19:22
 Operator : JC/MD
 Sample : N4991-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BT2

Quant Time: Oct 13 01:42:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 13 01:37:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	179264	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	200636	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	67658	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	83241	5.757	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	115.200%
7) Chloroethane-d5	1.909	69	62326	5.016	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.400%
11) 1,1-Dichloroethene-d2	2.562	65	31056	5.433	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	108.600%
20) 2-Butanone-d5	4.642	46	146316	45.958	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.920%
24) Chloroform-d	5.060	84	125482	4.655	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.000%
26) 1,2-Dichloroethane-d4	5.700	65	67900	4.884	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.600%
32) Benzene-d6	5.726	84	230561	4.177	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.600%
36) 1,2-Dichloropropane-d6	6.690	67	80398	4.289	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.800%
41) Toluene-d8	7.896	98	164706	3.335	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	66.800%#
43) trans-1,3-Dichloroprop...	8.179	79	22923	3.722	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.400%
46) 2-Hexanone-d5	8.636	63	75871	36.554	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	73.100%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	62323	4.162	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.200%
66) 1,2-Dichlorobenzene-d4	12.192	152	49796	4.234	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	84.600%
Target Compounds						
					Qvalue	
13) Acetone	2.662	43	9424	3.947	ug/L	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
Data File : VU051399.D
Acq On : 12 Oct 2022 19:22
Operator : JC/MD
Sample : N4991-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BT2

Quant Time: Oct 13 01:42:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 13 01:37:29 2022
Response via : Initial Calibration

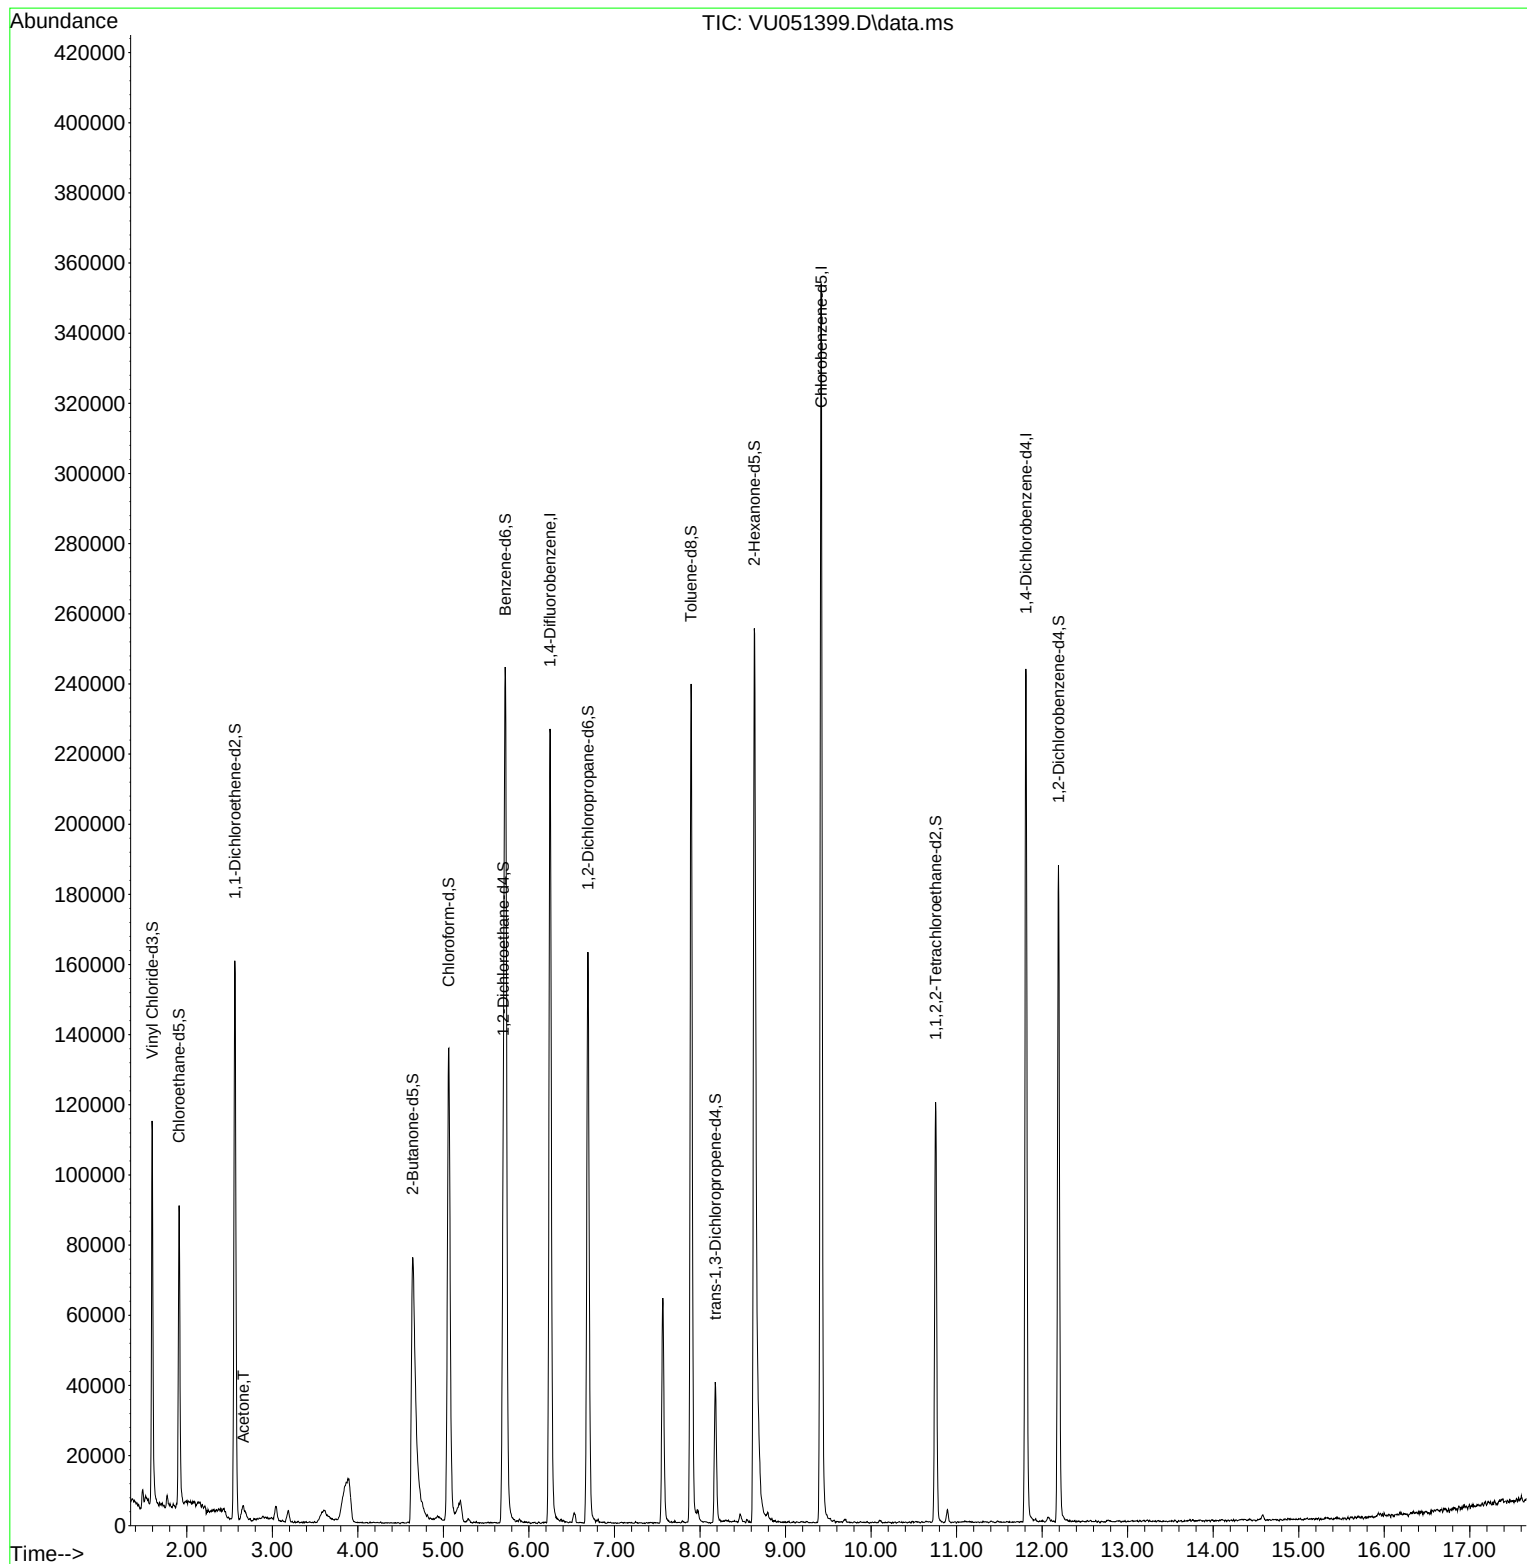

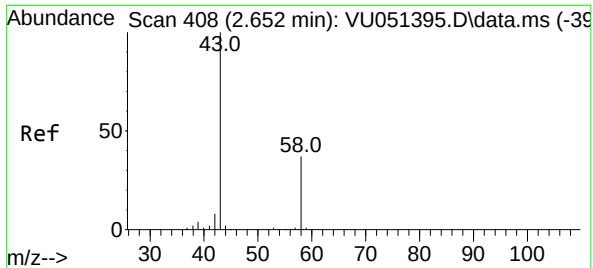

#13
 Acetone
 Concen: 3.947 ug/L
 RT: 2.662 min Scan# 411
 Delta R.T. 0.035 min
 Lab File: VU051399.D
 Acq: 12 Oct 2022 19:22

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BT2

Tgt Ion: 43 Resp: 9424
 Ion Ratio Lower Upper
 43 100
 58 21.3 0.0 68.8

