

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
 Data File : VU051390.D
 Acq On : 12 Oct 2022 14:25
 Operator : JC/MD
 Sample : N4993-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS13

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051390.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	72	79	93	rBV	108499	128093	20.24%	2.191%
2	1.909	169	177	190	rVB	84316	109407	17.28%	1.872%
3	2.562	369	380	398	rVB	156351	260985	41.23%	4.465%
4	3.829	750	774	779	rBV	6851	21409	3.38%	0.366%
5	3.864	782	785	806	rVB4	6678	12619	1.99%	0.216%
6	4.633	1012	1024	1060	rBV	76389	238458	37.67%	4.080%
7	5.064	1139	1158	1178	rBV3	130688	327864	51.80%	5.609%
8	5.176	1186	1193	1210	rVB	5792	14643	2.31%	0.251%
9	5.723	1343	1363	1390	rBV2	239880	623667	98.53%	10.670%
10	6.247	1509	1526	1555	rBV	236718	462214	73.02%	7.908%
11	6.539	1604	1617	1632	rBV4	27632	54123	8.55%	0.926%
12	6.691	1650	1664	1683	rBV	159077	312306	49.34%	5.343%
13	7.565	1924	1936	1950	rBV	65645	116894	18.47%	2.000%
14	7.896	2026	2039	2055	rBV	245551	423028	66.83%	7.237%
15	8.179	2115	2127	2143	rBV2	40785	70074	11.07%	1.199%
16	8.552	2228	2243	2258	rBV	296610	508131	80.27%	8.693%
17	8.636	2258	2269	2300	rVV3	228835	513019	81.05%	8.777%
18	9.414	2497	2511	2535	rBV	375797	632996	100.00%	10.829%
19	10.755	2916	2928	2948	rBV2	111935	184385	29.13%	3.154%
20	11.809	3244	3256	3280	rBV	298368	486029	76.78%	8.315%
21	12.192	3360	3375	3401	rBV	204752	344869	54.48%	5.900%




Sum of corrected areas: 5845213

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
Data File : VU051390.D
Acq On : 12 Oct 2022 14:25
Operator : JC/MD
Sample : N4993-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

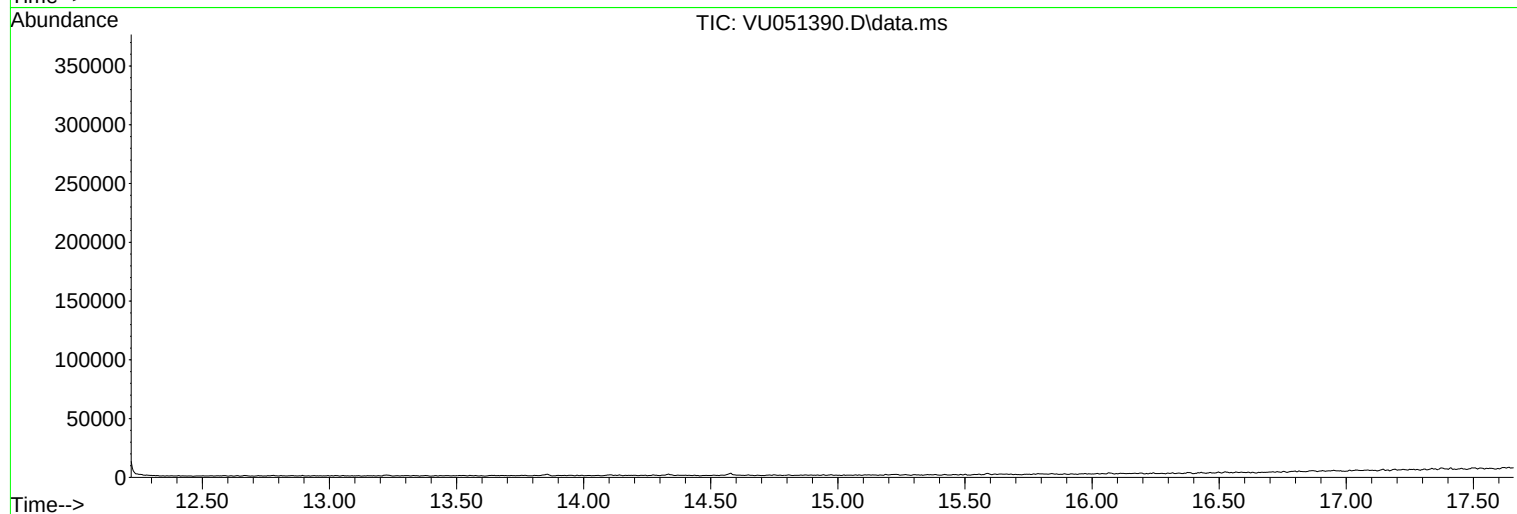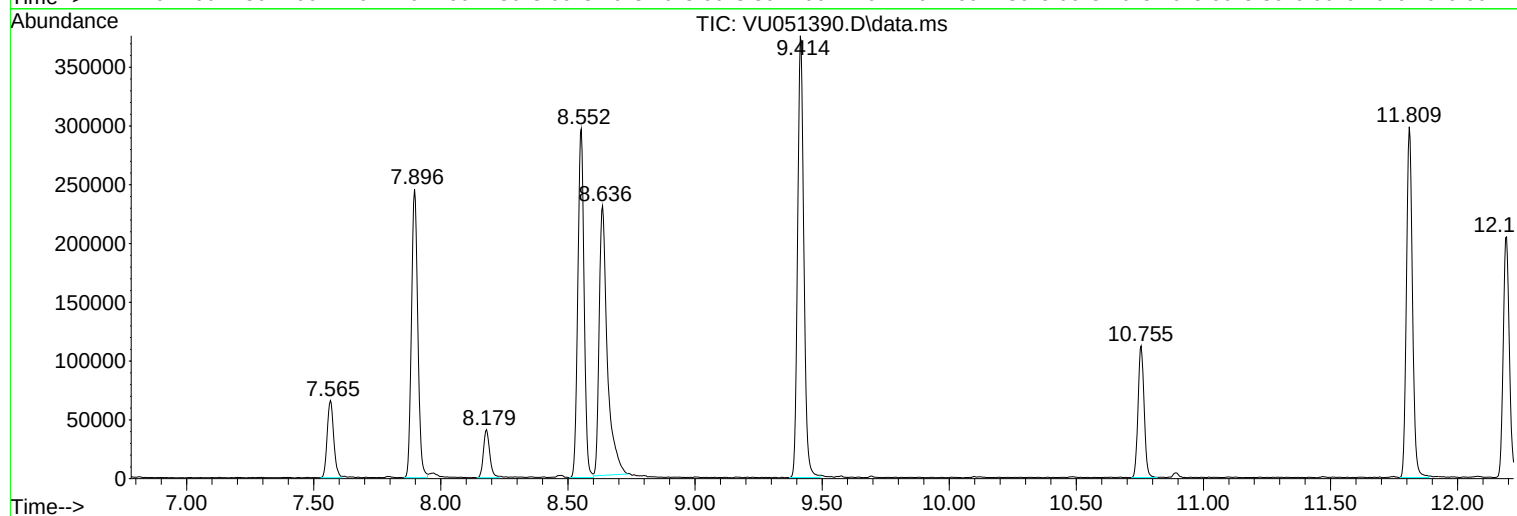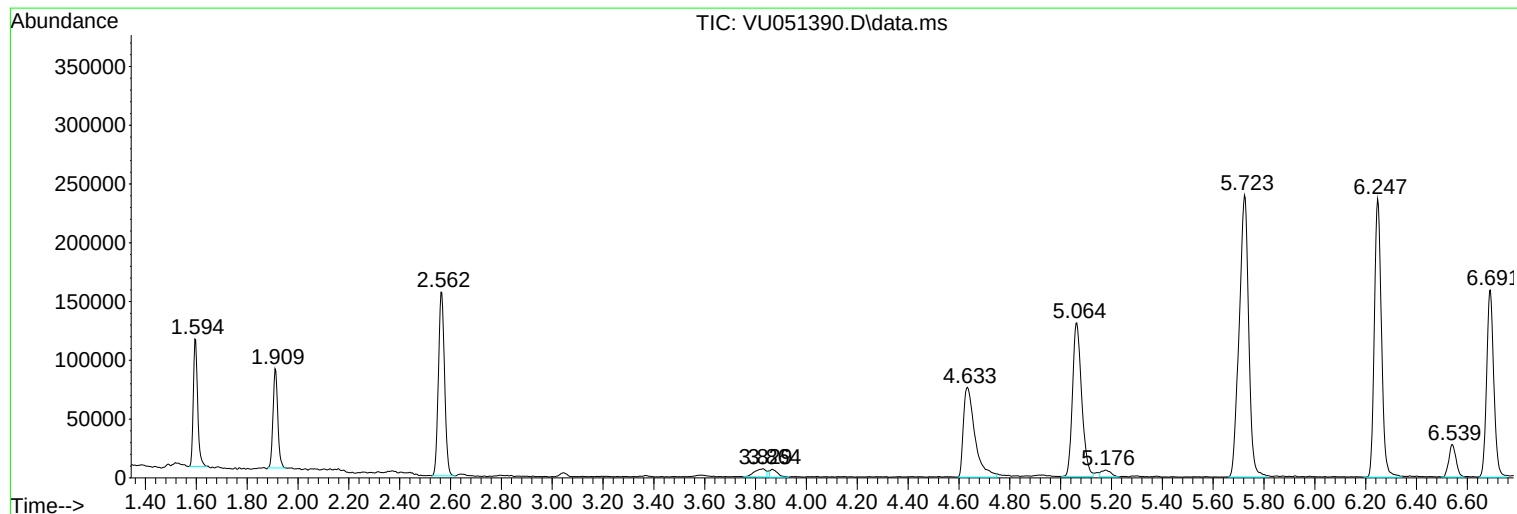

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
Data File : VU051390.D
Acq On : 12 Oct 2022 14:25
Operator : JC/MD
Sample : N4993-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
Data File : VU051390.D
Acq On : 12 Oct 2022 14:25
Operator : JC/MD
Sample : N4993-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc