

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
 Data File : VU051393.D
 Acq On : 12 Oct 2022 15:40
 Operator : JC/MD
 Sample : N4993-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS16

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051393.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	72	79	95	rVB	110169	132922	19.90%	2.410%
2	1.909	169	177	193	rBV	86771	113247	16.95%	2.054%
3	2.562	368	380	396	rBV	168734	285321	42.71%	5.174%
4	3.867	760	786	790	rBV2	9749	33457	5.01%	0.607%
5	4.639	1012	1026	1065	rBV2	87230	323174	48.37%	5.860%
6	5.063	1142	1158	1179	rBV2	133585	312441	46.77%	5.666%
7	5.186	1181	1196	1212	rVB	6209	20886	3.13%	0.379%
8	5.723	1340	1363	1394	rBV2	254430	668105	100.00%	12.115%
9	6.247	1511	1526	1547	rBV	225274	430979	64.51%	7.815%
10	6.542	1605	1618	1633	rBV5	22224	43945	6.58%	0.797%
11	6.690	1650	1664	1684	rBV	164018	327175	48.97%	5.933%
12	7.565	1921	1936	1955	rBV	68976	123472	18.48%	2.239%
13	7.896	2026	2039	2053	rBV	251788	437581	65.50%	7.935%
14	8.179	2115	2127	2146	rBV	43026	75195	11.25%	1.364%
15	8.636	2254	2269	2307	rBV2	278404	629188	94.18%	11.410%
16	9.417	2497	2512	2533	rBV	350328	587968	88.01%	10.662%
17	10.755	2912	2928	2948	rBV	127968	207242	31.02%	3.758%
18	10.893	2960	2971	2981	rBV2	5991	9675	1.45%	0.175%
19	11.809	3244	3256	3274	rBV	257885	419274	62.76%	7.603%
20	12.192	3362	3375	3401	rBV	198487	333349	49.89%	6.045%




Sum of corrected areas: 5514596

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
Data File : VU051393.D
Acq On : 12 Oct 2022 15:40
Operator : JC/MD
Sample : N4993-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

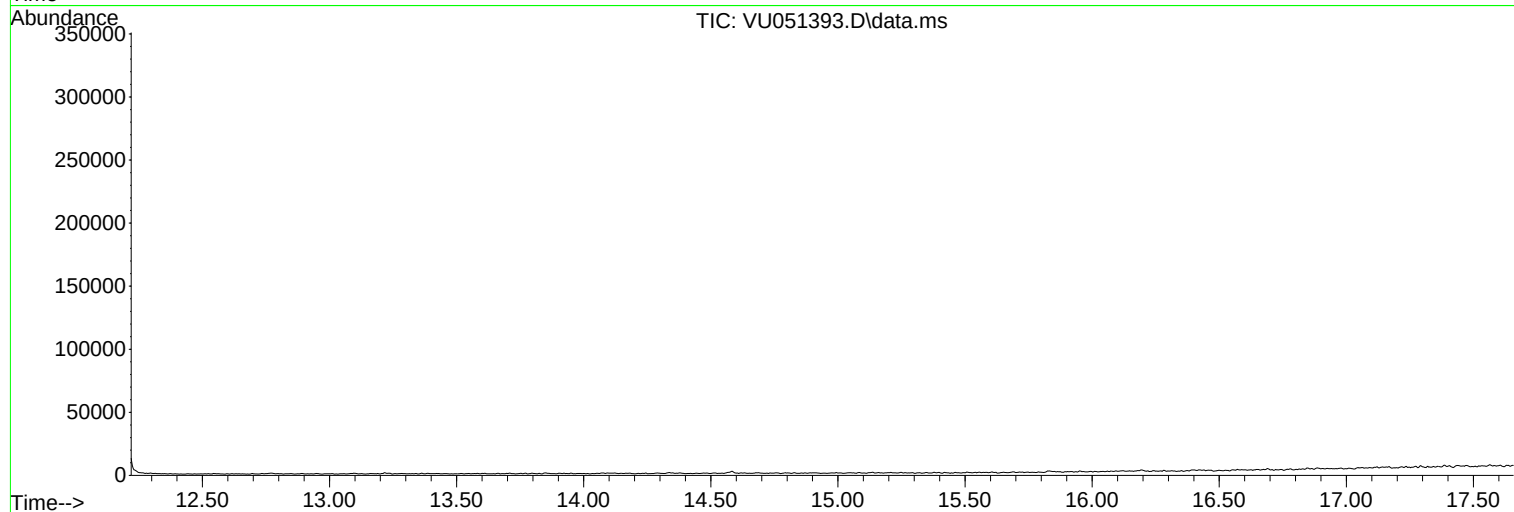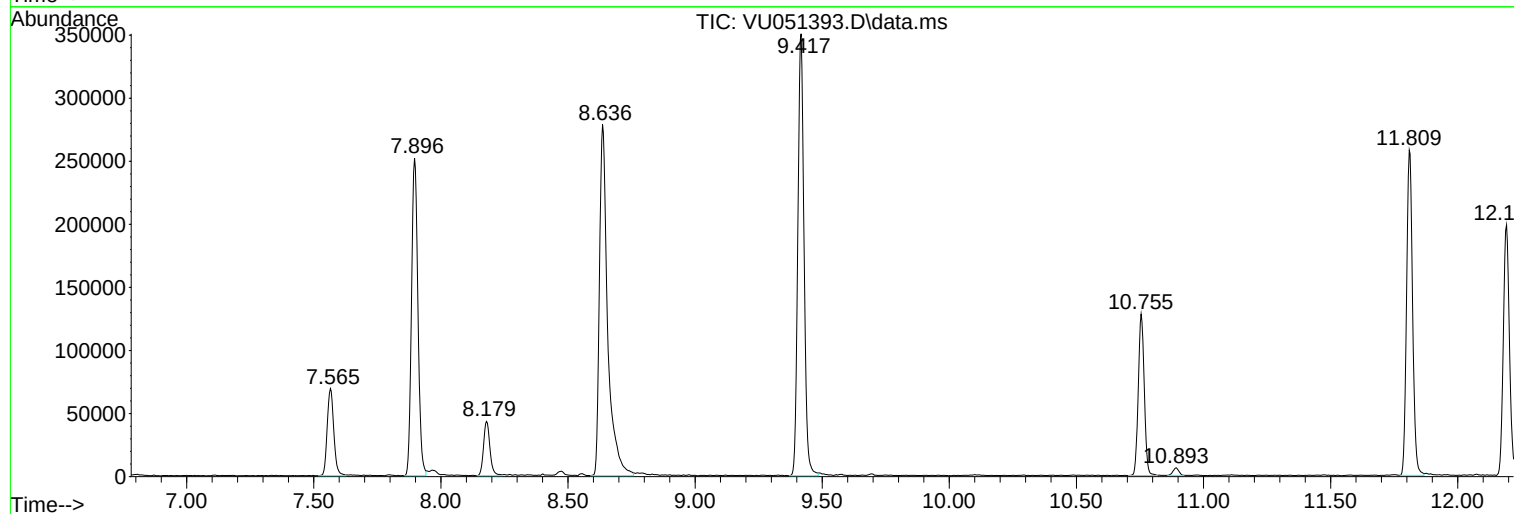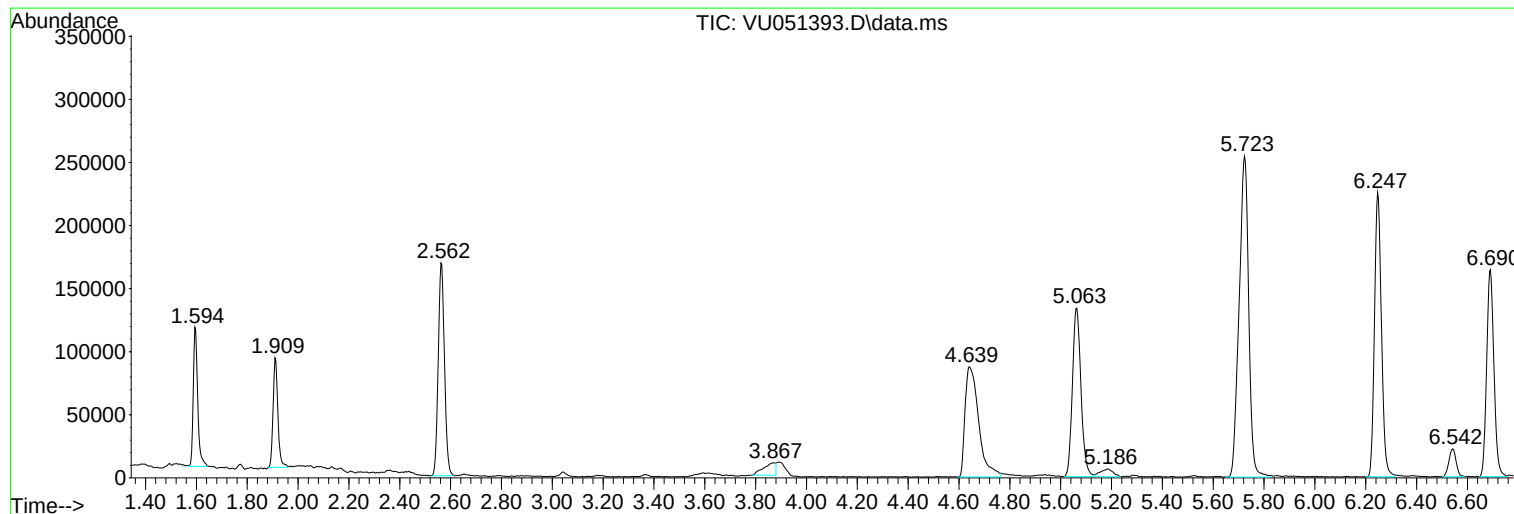

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
Data File : VU051393.D
Acq On : 12 Oct 2022 15:40
Operator : JC/MD
Sample : N4993-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
Data File : VU051393.D
Acq On : 12 Oct 2022 15:40
Operator : JC/MD
Sample : N4993-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc