

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
 Data File : VU051397.D
 Acq On : 12 Oct 2022 18:33
 Operator : JC/MD
 Sample : N5070-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BS7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051399.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	72	79	103	rVB	117243	140362	20.75%	2.570%
2	1.909	169	177	191	rBV	88911	115349	17.05%	2.112%
3	2.562	368	380	396	rBV	163410	263699	38.99%	4.829%
4	3.044	519	530	541	rVB7	3612	6982	1.03%	0.128%
5	3.189	563	575	585	rBV3	3511	7588	1.12%	0.139%
6	3.832	752	775	779	rBV	8317	24874	3.68%	0.456%
7	4.639	1010	1026	1066	rBV2	84707	288630	42.67%	5.286%
8	5.060	1141	1157	1178	rBV	138945	314827	46.55%	5.765%
9	5.723	1340	1363	1395	rBV3	259234	676345	100.00%	12.386%
10	6.247	1509	1526	1548	rBV	232565	444610	65.74%	8.142%
11	6.690	1650	1664	1685	rBV	172062	334780	49.50%	6.131%
12	7.565	1924	1936	1956	rBV	68692	123149	18.21%	2.255%
13	7.896	2026	2039	2057	rBV	250376	440335	65.11%	8.064%
14	8.179	2117	2127	2147	rBV2	41085	72240	10.68%	1.323%
15	8.472	2204	2218	2228	rBV4	5487	9870	1.46%	0.181%
16	8.636	2257	2269	2301	rBV3	277109	627982	92.85%	11.500%
17	9.417	2499	2512	2533	rBV	359959	604316	89.35%	11.067%
18	10.754	2913	2928	2948	rBV	129723	209813	31.02%	3.842%
19	10.893	2960	2971	2984	rBV	10813	17152	2.54%	0.314%
20	11.809	3245	3256	3275	rBV	249914	411220	60.80%	7.531%
21	12.192	3363	3375	3393	rBV2	199355	326450	48.27%	5.978%




Sum of corrected areas: 5460573

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
Data File : VU051397.D
Acq On : 12 Oct 2022 18:33
Operator : JC/MD
Sample : N5070-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

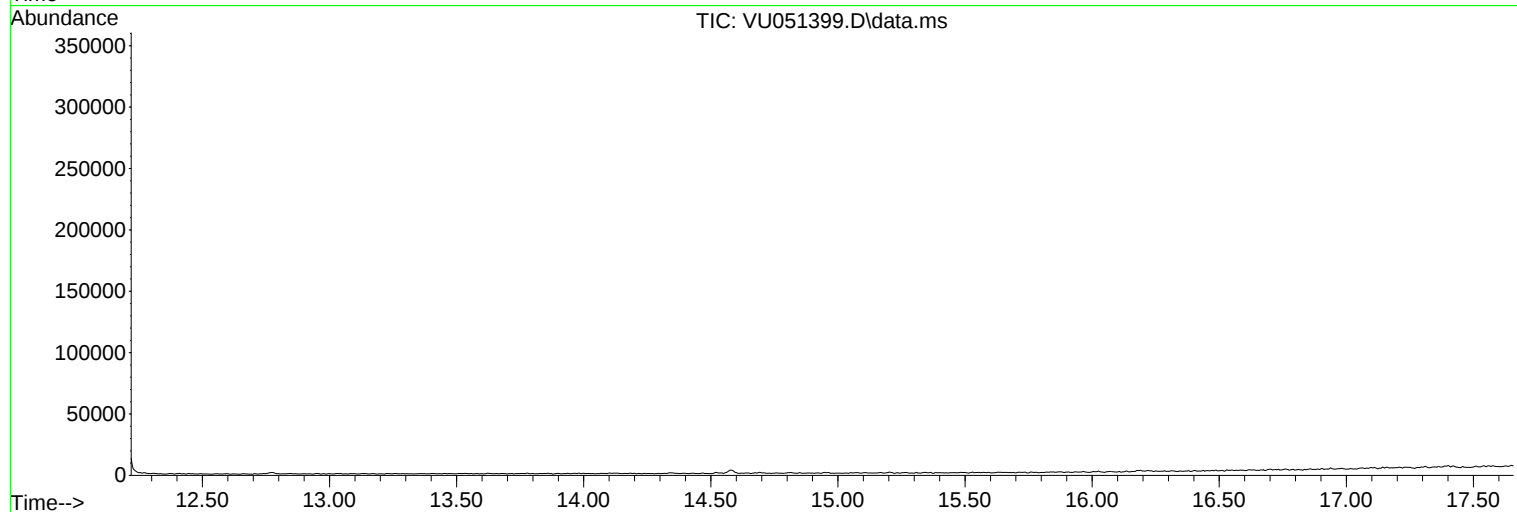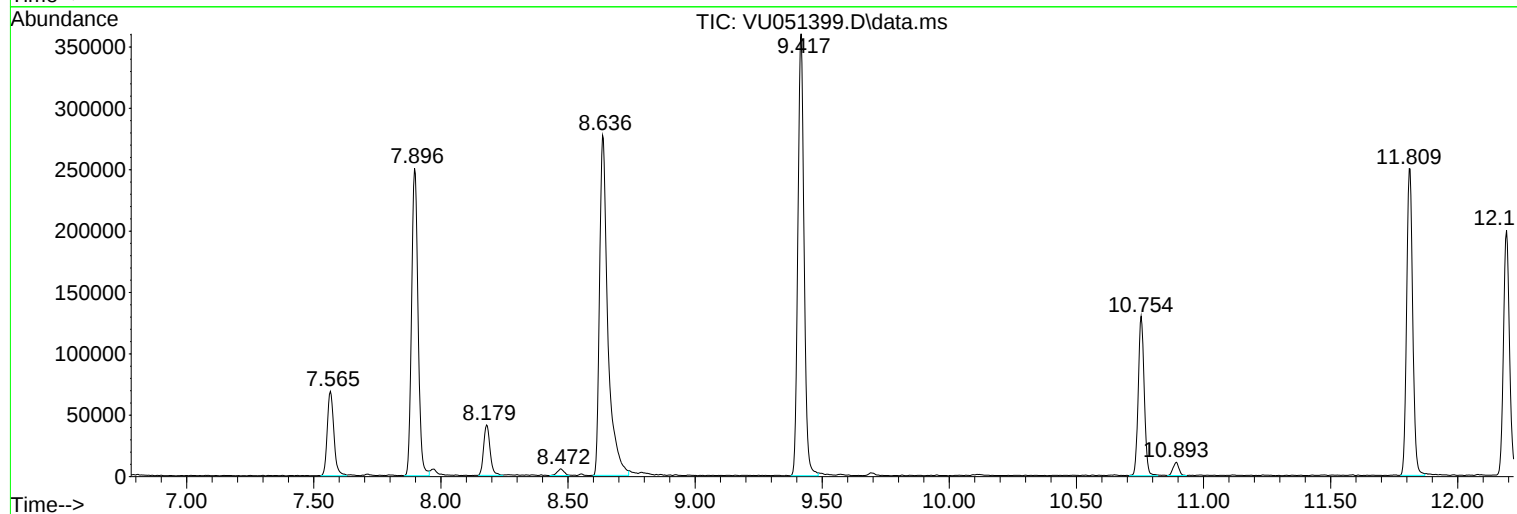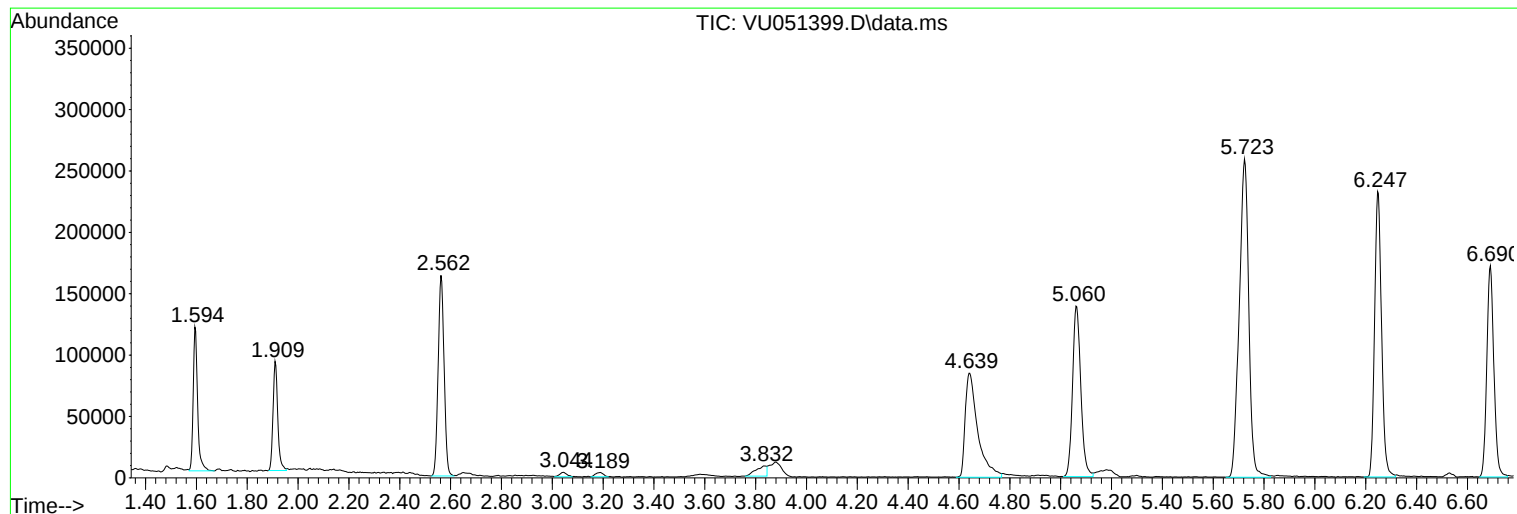

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
Data File : VU051397.D
Acq On : 12 Oct 2022 18:33
Operator : JC/MD
Sample : N5070-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
Data File : VU051397.D
Acq On : 12 Oct 2022 18:33
Operator : JC/MD
Sample : N5070-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc