

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
 Data File : VU051398.D
 Acq On : 12 Oct 2022 18:58
 Operator : JC/MD
 Sample : N5070-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BT7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU051400.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	72	79	94	rBV	112515	134710	20.37%	2.484%
2	1.909	168	177	191	rBV	90491	122623	18.54%	2.261%
3	2.562	368	380	398	rBV	161270	263595	39.85%	4.861%
4	3.041	517	529	547	rBV	39890	74436	11.25%	1.373%
5	4.639	1011	1026	1056	rBV2	84416	273740	41.39%	5.048%
6	5.063	1141	1158	1177	rBV	134459	296382	44.81%	5.465%
7	5.189	1178	1197	1198	rBV	4434	9125	1.38%	0.168%
8	5.722	1341	1363	1381	rBV2	254156	661397	100.00%	12.196%
9	6.247	1512	1526	1554	rBV	227949	446886	67.57%	8.241%
10	6.690	1650	1664	1682	rBV	168914	328962	49.74%	6.066%
11	7.565	1925	1936	1955	rBV2	66858	120784	18.26%	2.227%
12	7.896	2026	2039	2057	rBV	251617	435040	65.78%	8.022%
13	8.179	2116	2127	2143	rBV2	41395	71549	10.82%	1.319%
14	8.471	2209	2218	2232	rVB4	4558	8722	1.32%	0.161%
15	8.635	2256	2269	2305	rBV3	265267	613285	92.73%	11.309%
16	9.417	2499	2512	2538	rBV	354265	605305	91.52%	11.162%
17	10.754	2916	2928	2947	rBV2	126252	205185	31.02%	3.784%
18	10.893	2961	2971	2980	rBV2	9262	13708	2.07%	0.253%
19	11.812	3244	3257	3276	rBV	250711	417217	63.08%	7.694%
20	12.192	3363	3375	3392	rBV	193748	320257	48.42%	5.906%




Sum of corrected areas: 5422908

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
Data File : VU051398.D
Acq On : 12 Oct 2022 18:58
Operator : JC/MD
Sample : N5070-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

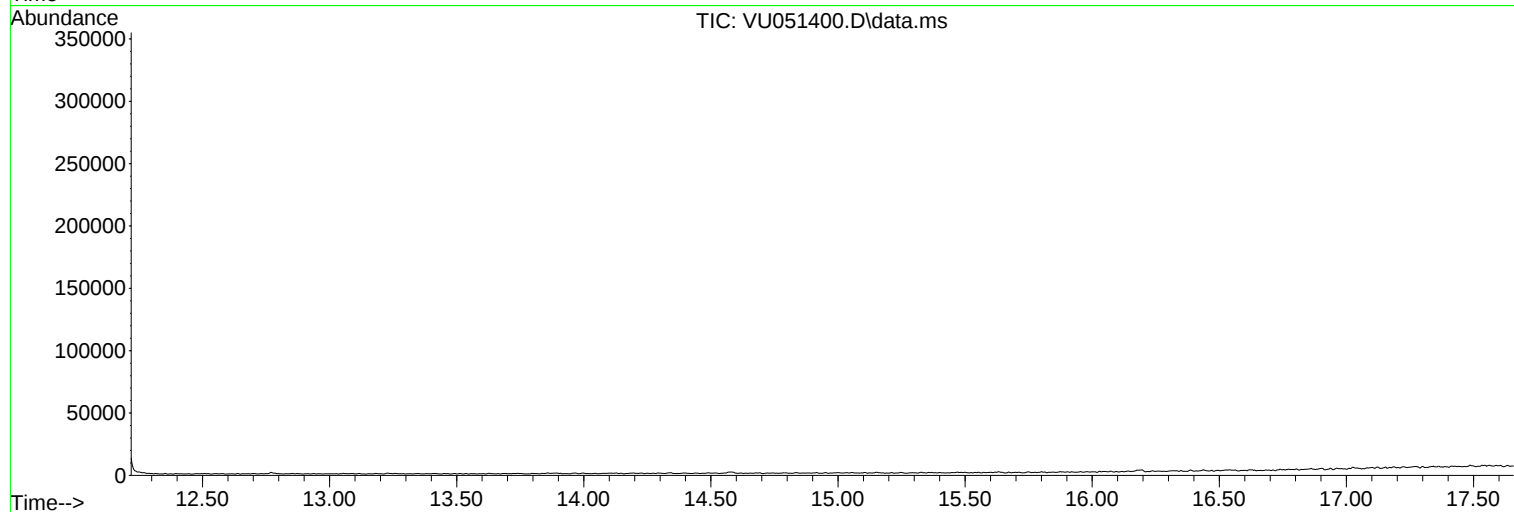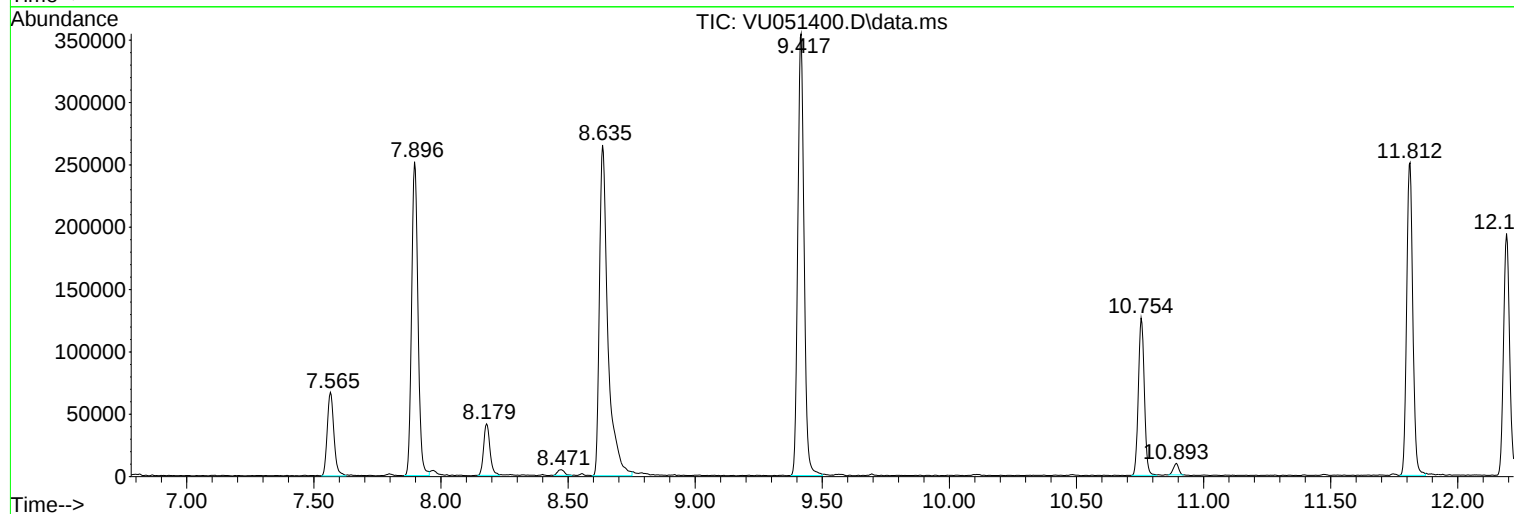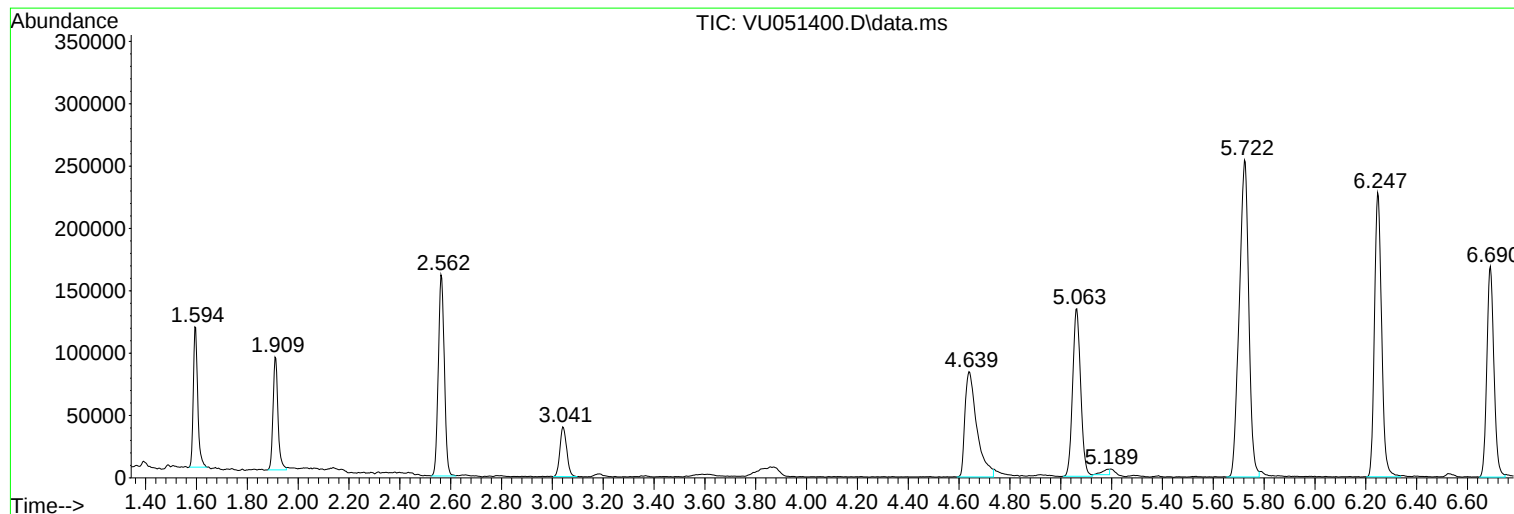

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
Data File : VU051398.D
Acq On : 12 Oct 2022 18:58
Operator : JC/MD
Sample : N5070-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
Data File : VU051398.D
Acq On : 12 Oct 2022 18:58
Operator : JC/MD
Sample : N5070-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc