

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
 Data File : VU051400.D
 Acq On : 12 Oct 2022 19:47
 Operator : JC/MD
 Sample : N5024-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BT3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051402.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	72	79	101	rVB	121270	146625	21.59%	2.646%
2	1.909	169	177	196	rBV	90856	118928	17.51%	2.146%
3	2.562	368	380	398	rBV	178262	287218	42.29%	5.183%
4	3.044	517	530	545	rVB	40700	76121	11.21%	1.374%
5	3.186	560	574	586	rVB2	3570	8277	1.22%	0.149%
6	3.838	753	777	779	rBV	7077	17450	2.57%	0.315%
7	4.642	1012	1027	1063	rBV2	81791	281443	41.44%	5.078%
8	5.060	1142	1157	1178	rBV	136360	302271	44.51%	5.454%
9	5.723	1343	1363	1392	rBV3	259758	679175	100.00%	12.255%
10	6.247	1513	1526	1544	rBV	230452	446333	65.72%	8.054%
11	6.690	1645	1664	1687	rBV	171884	336795	49.59%	6.077%
12	7.565	1923	1936	1953	rBV	67638	122185	17.99%	2.205%
13	7.896	2026	2039	2056	rBV	255197	446119	65.69%	8.050%
14	8.179	2111	2127	2145	rBV2	43791	75155	11.07%	1.356%
15	8.469	2206	2217	2233	rBV3	3585	7652	1.13%	0.138%
16	8.636	2257	2269	2310	rBV3	265228	618695	91.10%	11.164%
17	9.417	2498	2512	2531	rBV	363743	613300	90.30%	11.067%
18	10.755	2915	2928	2948	rBV	126548	208730	30.73%	3.766%
19	10.893	2961	2971	2984	rVB2	4636	7758	1.14%	0.140%
20	11.812	3244	3257	3278	rBV	254159	417669	61.50%	7.537%
21	12.192	3361	3375	3392	rBV	195209	323959	47.70%	5.846%




Sum of corrected areas: 5541858

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
Data File : VU051400.D
Acq On : 12 Oct 2022 19:47
Operator : JC/MD
Sample : N5024-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

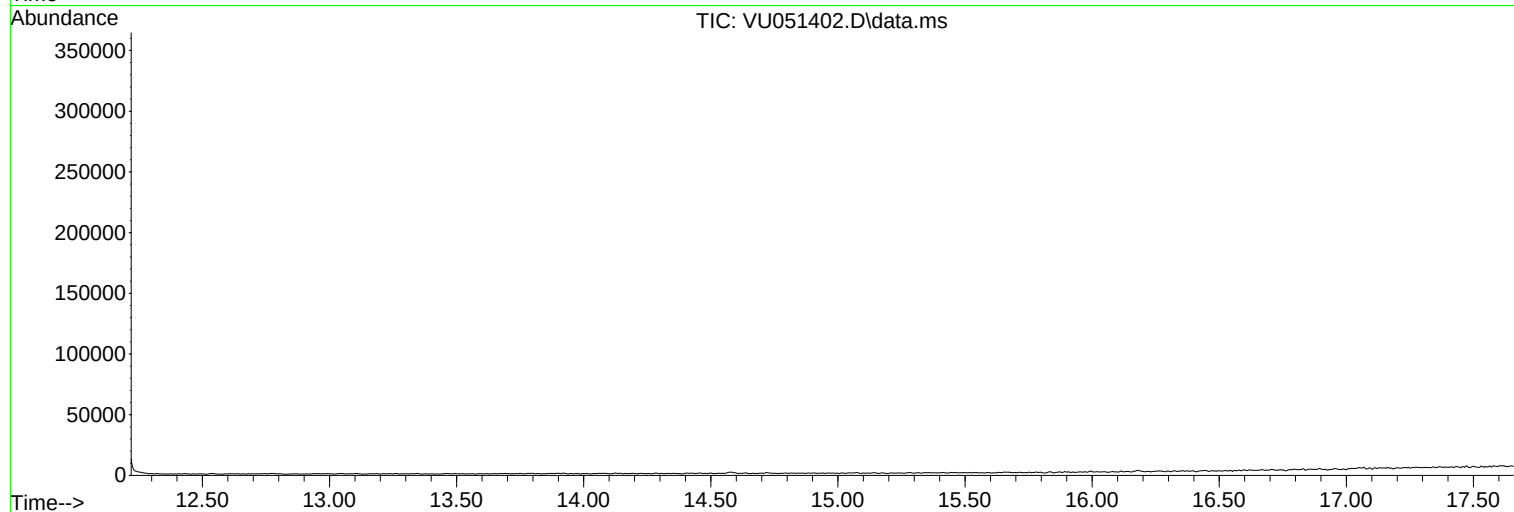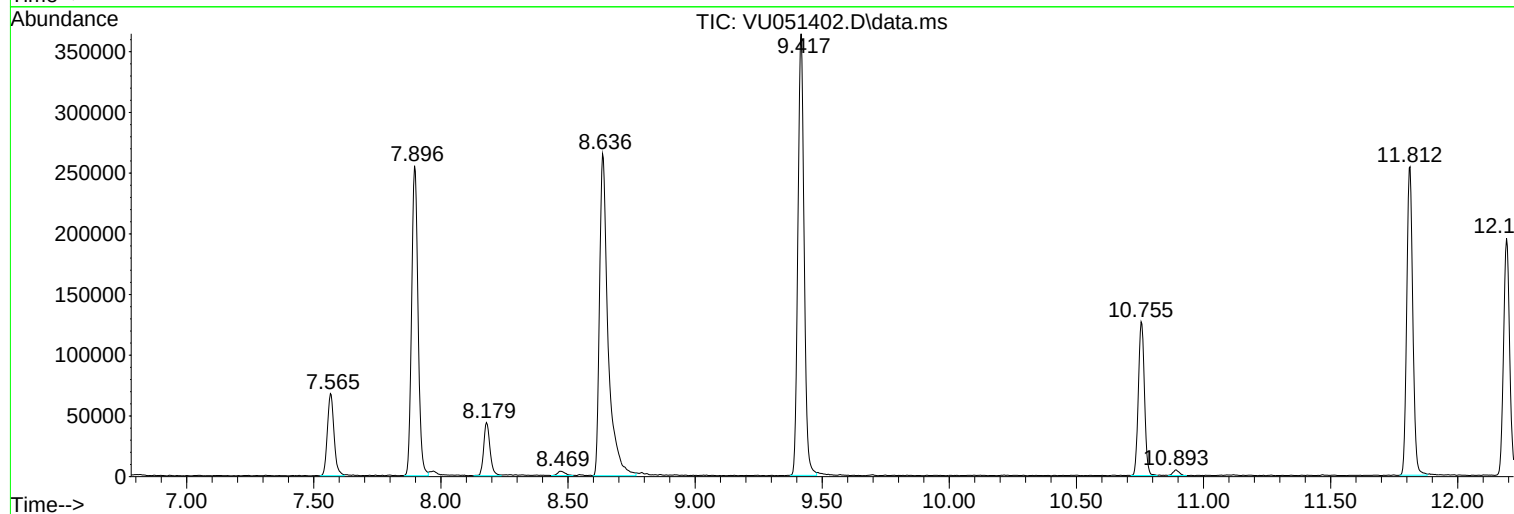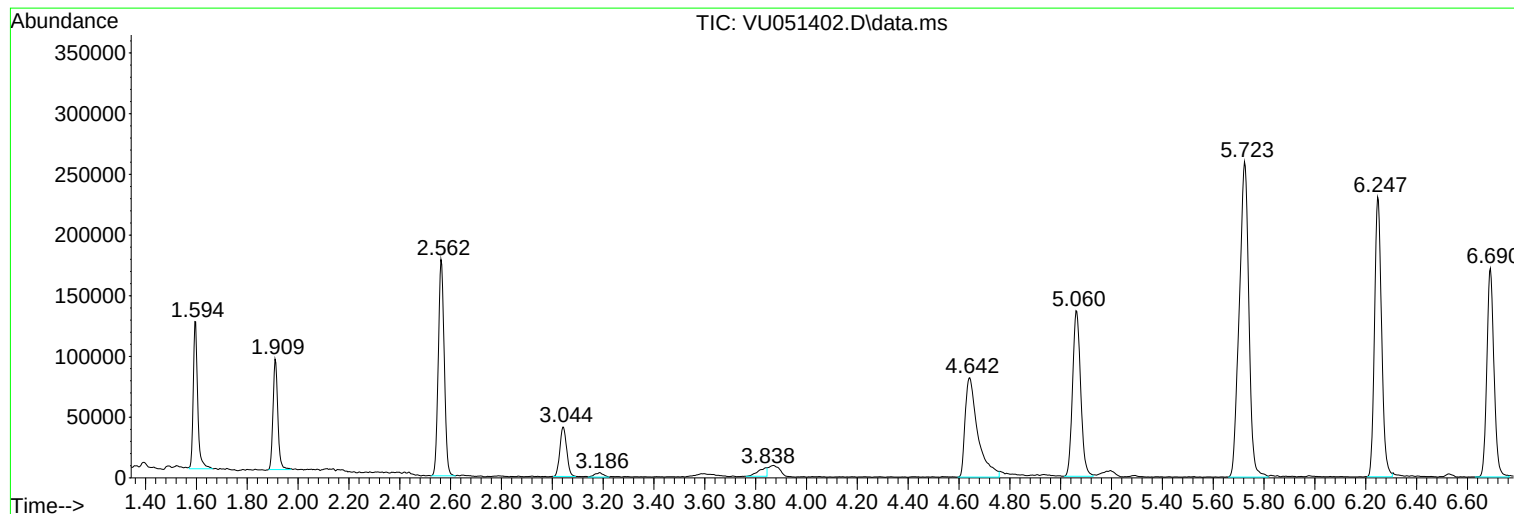

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
Data File : VU051400.D
Acq On : 12 Oct 2022 19:47
Operator : JC/MD
Sample : N5024-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
Data File : VU051400.D
Acq On : 12 Oct 2022 19:47
Operator : JC/MD
Sample : N5024-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc