
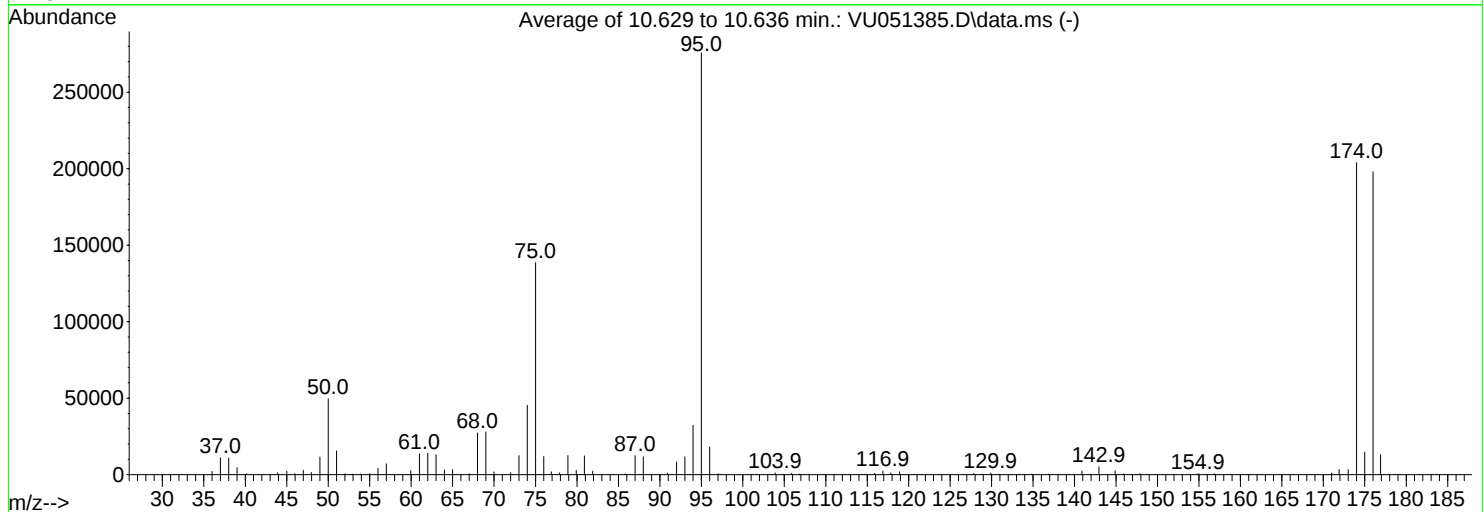


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101222\
 Data File : VU051385.D
 Acq On : 12 Oct 2022 09:47
 Operator : JC/MD
 Sample : BFB155
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB155

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Oct 13 01:37:29 2022

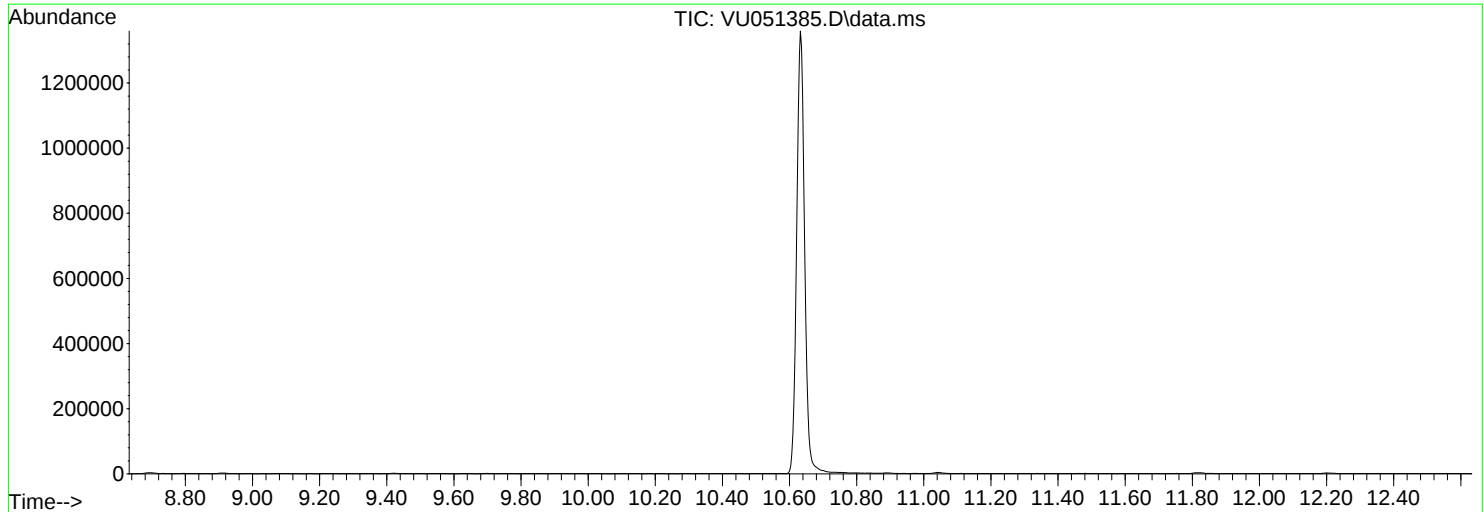

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	49629	PASS
75	95	30	80	50.3	138645	PASS
95	95	100	100	100.0	275733	PASS
96	95	5	9	6.6	18107	PASS
173	174	0.00	2	1.6	3290	PASS
174	95	50	120	74.0	203925	PASS
175	174	5	9	7.2	14720	PASS
176	174	95	101	97.1	198016	PASS
177	176	5	9	6.6	13047	PASS

m/z	Abundance
39.90	260.0
43.90	601.0

Instrument :
MSVOA_U
ClientSampleId :
BFB155

m/z	Abundance
36.00	2104.0
37.00	11330.0
38.00	10797.0
39.00	4406.0
40.10	620.0
43.20	111.0
43.90	1674.0
45.00	2163.0
46.00	727.0
47.00	2958.0
48.00	1527.0
49.00	11300.0
50.00	49328.0
51.00	15681.0
52.10	723.0
52.90	460.0
53.90	439.0
55.00	763.0
56.00	4117.0
57.00	6887.0
57.90	261.0
60.00	2607.0
61.00	13533.0
62.00	13830.0
63.00	13465.0
64.00	3184.0
65.00	3150.0
66.00	285.0
67.00	624.0
68.00	26840.0
69.00	27576.0
70.00	1806.0
72.00	1382.0
73.00	12184.0
74.00	44552.0
75.00	135232.0
76.00	11677.0
76.90	1949.0
77.90	1180.0
78.90	12277.0
79.90	2856.0
80.90	12458.0
81.90	2276.0
83.00	211.0
85.80	513.0
87.00	11917.0
88.00	11255.0
90.90	1017.0
92.00	7990.0
93.00	11364.0
94.00	31688.0
95.00	269696.0
96.00	17640.0
97.00	535.0
103.00	143.0
103.90	1171.0
104.80	315.0
105.90	976.0
106.90	242.0
108.00	365.0
110.00	125.0
110.90	204.0
112.00	165.0
112.80	180.0
114.90	304.0
115.90	1064.0
116.90	2347.0
117.80	1122.0
118.90	1978.0
119.90	113.0
123.80	100.0
126.00	162.0
127.80	729.0
128.80	403.0
129.90	910.0
130.80	372.0
134.80	402.0
136.90	452.0
139.90	187.0
140.90	2279.0
141.90	340.0
143.00	5232.0
144.00	256.0
144.90	2739.0
145.90	486.0
146.80	167.0
147.90	566.0
148.70	206.0
149.80	205.0
151.90	156.0
152.90	124.0
153.80	189.0

Instrument :
MSVOA_U
ClientSampleId :
BFB155

154.90	681.0
155.90	140.0
156.90	552.0
158.00	100.0
158.80	350.0
160.80	247.0
171.00	1144.0
171.90	3278.0
173.00	3304.0
174.00	195072.0
175.00	14839.0
176.00	189056.0
176.90	12669.0
177.90	320.0

Instrument :
MSVOA_U
ClientSampleId :
BFB155

m/z	Abundance
36.00	2218.0
37.00	11127.0
38.00	11189.0
39.00	4714.0
40.20	652.0
43.00	107.0
43.90	1833.0
45.00	2401.0
46.00	678.0
47.00	3052.0
47.90	1592.0
49.00	12016.0
50.00	51112.0
51.00	15889.0
52.00	625.0
52.90	438.0
53.90	420.0
55.00	764.0
56.00	4346.0
57.00	7309.0
57.90	286.0
60.00	2653.0
61.00	14027.0
62.00	14353.0
63.00	13251.0
64.00	3107.0
65.00	3360.0
65.90	257.0
67.00	612.0
68.00	28400.0
69.00	28784.0
70.00	1859.0
71.10	107.0
72.00	1407.0
73.00	12864.0
74.00	46656.0
75.00	143360.0
76.00	12210.0
76.90	1924.0
77.90	1152.0
78.90	12856.0
79.90	2866.0
80.90	12541.0
81.90	2458.0
83.00	253.0
85.90	598.0
87.00	12916.0
88.00	11963.0
90.90	1113.0
92.00	8597.0
93.00	12039.0
94.00	33416.0
95.00	283840.0
96.00	18736.0
97.10	618.0
102.90	175.0
103.90	1161.0
104.80	337.0
105.90	1011.0
106.80	290.0
108.00	362.0
109.90	142.0
110.90	179.0
112.00	217.0
112.80	180.0
114.90	286.0
115.90	991.0
116.90	2467.0
117.80	1175.0
118.90	1965.0
123.80	152.0
125.90	169.0
127.80	826.0
128.80	467.0
129.90	1108.0
130.80	317.0
134.90	421.0
136.80	453.0
139.90	186.0
140.90	2392.0
141.90	304.0
143.00	5197.0
144.00	269.0
144.90	2723.0
145.90	532.0
146.90	223.0
147.90	641.0
148.70	258.0
149.80	288.0
151.90	151.0
152.90	161.0
153.90	214.0

Instrument :
MSVOA_U
ClientSampleId :
BFB155

154.90	733.0
155.90	146.0
156.90	582.0
158.80	353.0
160.80	232.0
171.00	1140.0
171.90	3440.0
173.00	3400.0
174.00	210176.0
175.00	15043.0
176.00	204352.0
176.90	13402.0
177.90	341.0

Instrument :
MSVOA_U
ClientSampleId :
BFB155

m/z	Abundance
36.00	2150.0
37.00	10557.0
38.00	10642.0
39.00	4596.0
40.20	619.0
43.00	169.0
44.00	1954.0
45.00	2321.0
45.90	612.0
47.00	2891.0
47.90	1436.0
49.00	11295.0
50.00	48448.0
51.00	14996.0
52.00	628.0
52.90	417.0
53.90	334.0
55.00	672.0
56.00	4035.0
57.00	7107.0
58.00	249.0
59.90	2509.0
61.00	13125.0
62.00	13852.0
63.00	12129.0
64.00	2890.0
65.00	3196.0
66.00	255.0
67.00	552.0
68.00	26760.0
69.00	27512.0
70.00	1813.0
71.00	124.0
72.00	1432.0
73.00	12347.0
74.00	44648.0
75.00	137344.0
76.00	11632.0
76.90	1757.0
77.90	1023.0
78.90	12324.0
79.90	2694.0
80.90	11687.0
81.90	2365.0
82.90	293.0
85.90	646.0
87.00	12572.0
88.00	11535.0
90.90	1074.0
92.00	8112.0
93.00	11604.0
94.00	31992.0
95.00	273664.0
96.00	17944.0
97.00	577.0
102.90	183.0
103.90	1212.0
104.90	379.0
105.90	988.0
106.80	293.0
107.90	316.0
109.90	168.0
110.90	157.0
112.00	236.0
112.80	161.0
114.80	242.0
115.90	904.0
116.90	2417.0
117.90	1103.0
118.90	1865.0
123.80	177.0
125.80	165.0
127.90	802.0
128.90	498.0
129.90	1173.0
130.90	307.0
134.90	419.0
136.80	436.0
139.90	160.0
140.90	2227.0
141.90	266.0
142.90	4856.0
144.00	229.0
144.90	2455.0
145.90	488.0
146.90	240.0
147.90	628.0
148.80	261.0
149.80	310.0
151.90	149.0
152.90	185.0
154.00	180.0

Instrument :
MSVOA_U
ClientSampleId :
BFB155

154.90	707.0
156.00	125.0
156.90	500.0
157.90	120.0
158.80	265.0
160.90	248.0
171.00	984.0
171.90	3345.0
173.00	3165.0
174.00	206528.0
175.00	14279.0
176.00	200640.0
176.90	13071.0
177.90	302.0

Instrument :
MSVOA_U
ClientSampleId :
BFB155