

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101223\
 Data File : VU055759.D
 Acq On : 12 Oct 2023 12:14
 Operator : MD/SY
 Sample : 04792-07DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY1B5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M

Title : VOC Analysis

Signal : TIC: VU055759.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	114	rBV	200222	237723	12.61%	1.570%
2	1.891	180	187	207	rVB	169763	243413	12.91%	1.608%
3	2.560	383	395	411	rBV	353854	584856	31.03%	3.863%
4	2.911	502	504	506	rBV	397	162	0.01%	0.001%
5	2.962	519	520	523	rVB3	393	185	0.01%	0.001%
6	3.036	534	543	555	rVB4	5586	9675	0.51%	0.064%
7	3.184	574	589	613	rVB2	13968	36140	1.92%	0.239%
8	3.325	626	633	635	rBV2	505	551	0.03%	0.004%
9	3.386	650	652	656	rBV2	393	226	0.01%	0.001%
10	3.431	664	666	671	rBV2	267	190	0.01%	0.001%
11	3.457	671	674	677	rBV	349	204	0.01%	0.001%
12	3.676	739	742	745	rBV2	382	216	0.01%	0.001%
13	3.718	753	755	760	rBV2	213	146	0.01%	0.001%
14	3.759	764	768	771	rBV2	325	301	0.02%	0.002%
15	3.804	780	782	785	rVB	207	110	0.01%	0.001%
16	3.820	785	787	795	rBV2	340	388	0.02%	0.003%
17	3.869	799	802	804	rBV	206	109	0.01%	0.001%
18	3.930	818	821	824	rVB2	344	224	0.01%	0.001%
19	3.952	824	828	836	rBV	349	389	0.02%	0.003%
20	4.010	840	846	850	rBV3	426	500	0.03%	0.003%
21	4.161	892	893	895	rBV	303	96	0.01%	0.001%
22	4.206	904	907	911	rBV	239	149	0.01%	0.001%
23	4.274	922	928	929	rBV	418	312	0.02%	0.002%
24	4.441	978	980	982	rBV	227	126	0.01%	0.001%
25	4.467	986	988	990	rBV	153	80	0.00%	0.001%
26	4.615	1023	1034	1061	rBV	144877	385728	20.46%	2.548%
27	5.058	1152	1172	1195	rBV	348356	774075	41.07%	5.113%
28	5.370	1266	1269	1273	rVB	438	233	0.01%	0.002%
29	5.390	1273	1275	1277	rBV	325	184	0.01%	0.001%
30	5.431	1285	1288	1292	rBV2	200	151	0.01%	0.001%
31	5.460	1292	1297	1302	rBV3	396	467	0.02%	0.003%
32	5.483	1302	1304	1309	rVB2	290	126	0.01%	0.001%
33	5.505	1309	1311	1314	rVB2	371	202	0.01%	0.001%
34	5.521	1314	1316	1317	rBV	447	204	0.01%	0.001%
35	5.721	1357	1378	1420	rBV2	675059	1884968	100.00%	12.451%
36	6.103	1495	1497	1498	rBV	258	93	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101223\
 Data File : VU055759.D
 Acq On : 12 Oct 2023 12:14
 Operator : MD/SY
 Sample : 04792-07DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY1B5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	6.190	1522	1524	1526	rBV	174	90	0.00%	0.001%
38	6.245	1528	1541	1579	rVV	563012	1090675	57.86%	7.204%
39	6.528	1618	1629	1644	rBV6	21829	46220	2.45%	0.305%
40	6.627	1658	1660	1664	rBV3	429	324	0.02%	0.002%
41	6.685	1664	1678	1699	rBV	435410	858021	45.52%	5.668%
42	6.869	1733	1735	1741	rVB4	643	491	0.03%	0.003%
43	6.920	1748	1751	1757	rVB3	646	548	0.03%	0.004%
44	6.946	1757	1759	1761	rBV	169	101	0.01%	0.001%
45	7.036	1785	1787	1789	rBV2	332	145	0.01%	0.001%
46	7.100	1804	1807	1808	rBV2	247	134	0.01%	0.001%
47	7.139	1816	1819	1820	rBV	203	82	0.00%	0.001%
48	7.152	1820	1823	1826	rVB2	329	209	0.01%	0.001%
49	7.197	1826	1837	1842	rBV3	3332	5584	0.30%	0.037%
50	7.242	1848	1851	1853	rBV2	411	214	0.01%	0.001%
51	7.479	1923	1925	1931	rVB2	319	253	0.01%	0.002%
52	7.508	1931	1934	1937	rBV2	441	290	0.02%	0.002%
53	7.563	1938	1951	1979	rBV	233582	418344	22.19%	2.763%
54	7.798	2021	2024	2026	rBV3	711	471	0.02%	0.003%
55	7.849	2038	2040	2041	rBV	431	190	0.01%	0.001%
56	7.894	2041	2054	2093	rVV	811164	1432238	75.98%	9.461%
57	8.177	2131	2142	2166	rBV2	164893	284895	15.11%	1.882%
58	8.380	2203	2205	2206	rBV	418	186	0.01%	0.001%
59	8.422	2215	2218	2219	rBV	264	132	0.01%	0.001%
60	8.505	2241	2244	2245	rBV2	503	288	0.02%	0.002%
61	8.550	2245	2258	2273	rVV	377009	645421	34.24%	4.263%
62	8.634	2274	2284	2327	rVB3	408371	997150	52.90%	6.587%
63	8.942	2377	2380	2383	rBV3	503	361	0.02%	0.002%
64	9.274	2482	2483	2487	rVB2	387	162	0.01%	0.001%
65	9.299	2489	2491	2495	rBV2	391	270	0.01%	0.002%
66	9.415	2514	2527	2557	rBV	837855	1405333	74.55%	9.283%
67	9.740	2626	2628	2630	rBV	427	191	0.01%	0.001%
68	9.811	2647	2650	2651	rBV	396	216	0.01%	0.001%
69	9.888	2671	2674	2678	rVB2	548	389	0.02%	0.003%
70	10.315	2804	2807	2809	rBV	417	292	0.02%	0.002%
71	10.753	2929	2943	2969	rBV	650725	1079085	57.25%	7.128%
72	11.142	3060	3064	3065	rBV	371	295	0.02%	0.002%
73	11.434	3153	3155	3156	rBV	294	95	0.01%	0.001%
74	11.753	3246	3254	3259	rBV6	1704	2384	0.13%	0.016%
75	11.810	3259	3272	3302	rBV	827715	1334736	70.81%	8.817%
76	12.193	3378	3391	3409	rBV	817236	1355675	71.92%	8.955%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101223\
Data File : VU055759.D
Acq On : 12 Oct 2023 12:14
Operator : MD/SY
Sample : 04792-07DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY1B5DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Title : VOC Analysis

77	12.675	3537	3541	3546	rVB3	548	605	0.03%	0.004%
78	12.708	3546	3551	3556	rBV3	814	976	0.05%	0.006%
79	13.855	3902	3908	3919	rVB6	3406	4762	0.25%	0.031%
80	14.106	3979	3986	3990	rBV3	5350	7537	0.40%	0.050%


Sum of corrected areas: 15138962

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101223\
Data File : VU055759.D
Acq On : 12 Oct 2023 12:14
Operator : MD/SY
Sample : 04792-07DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY1B5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

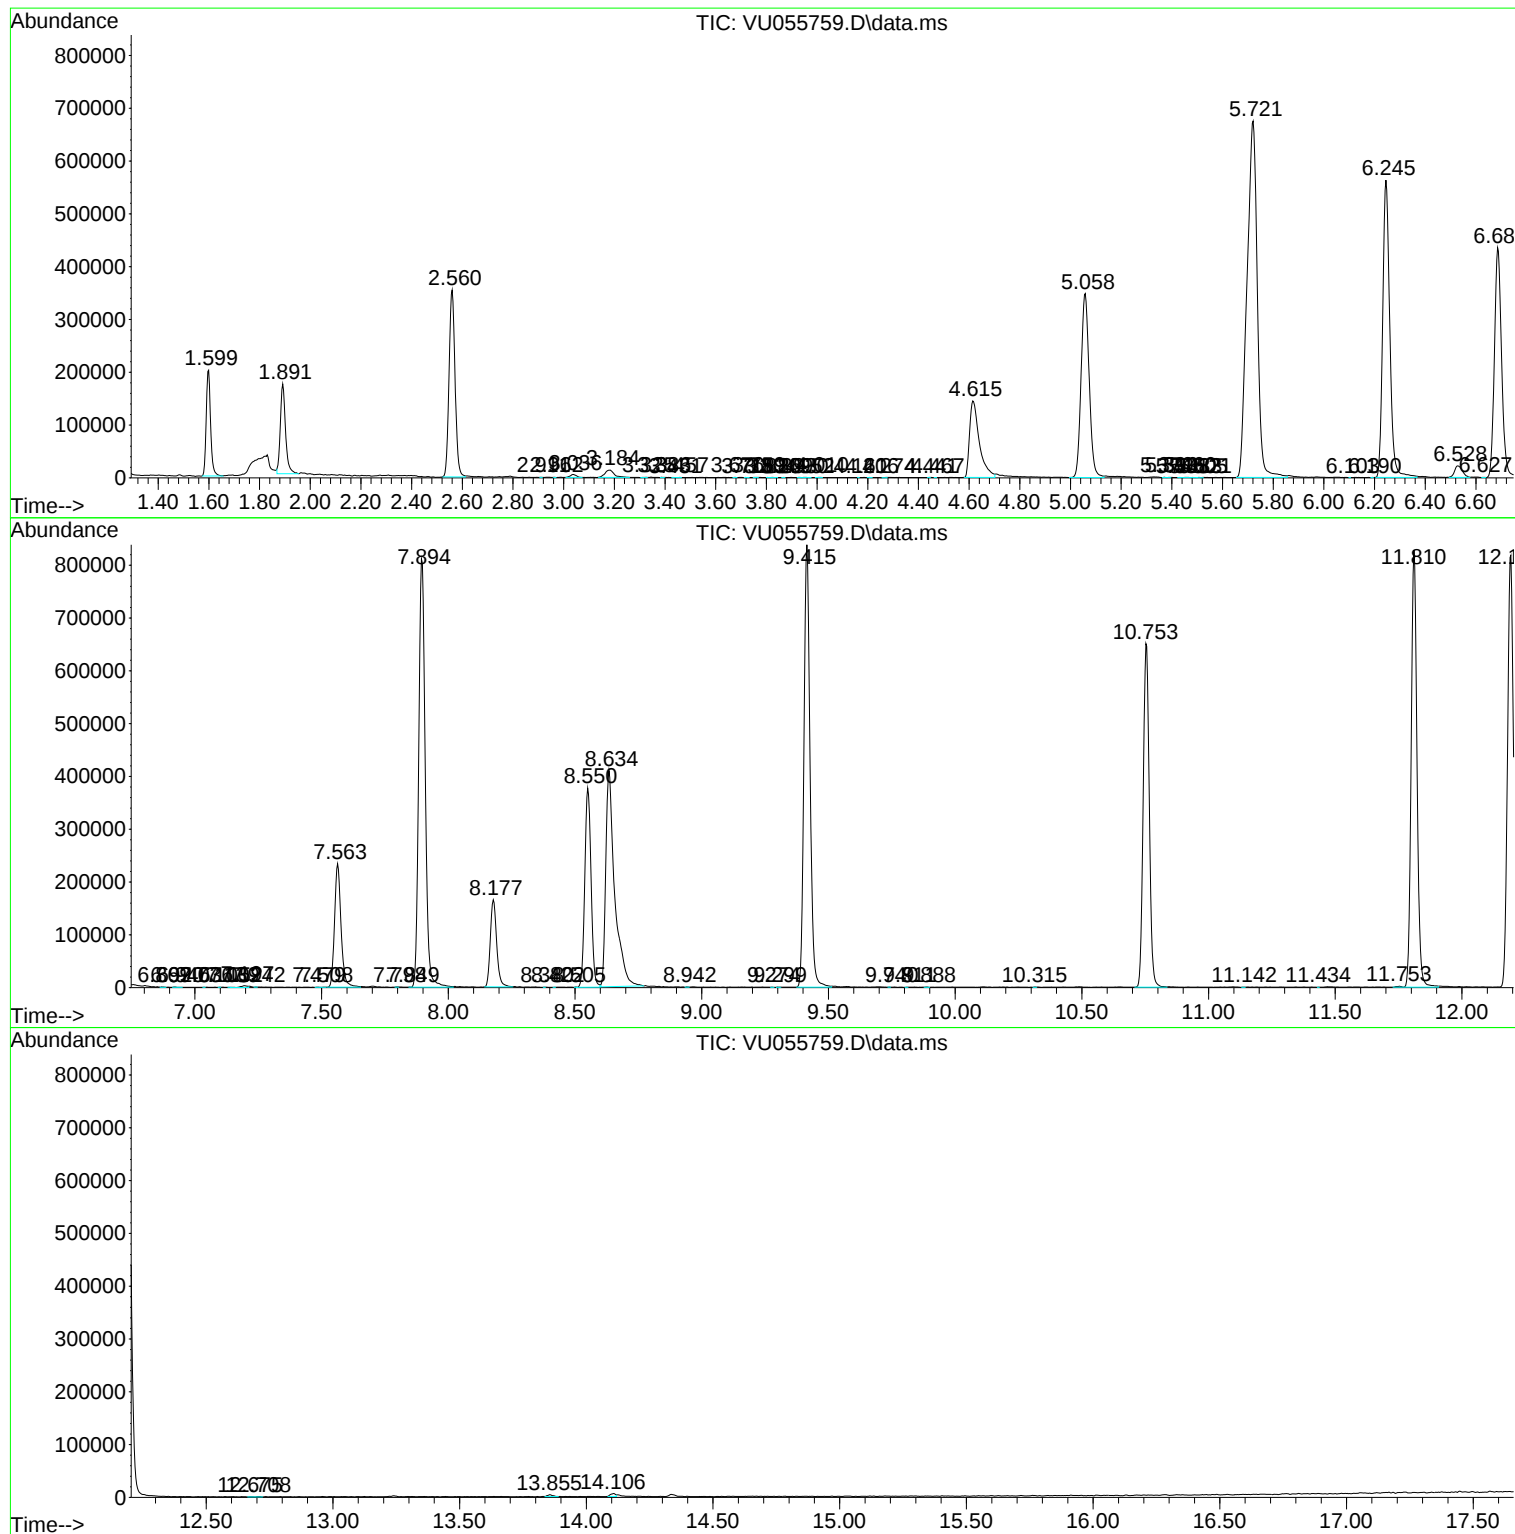

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101223\
Data File : VU055759.D
Acq On : 12 Oct 2023 12:14
Operator : MD/SY
Sample : 04792-07DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY1B5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101223\
Data File : VU055759.D
Acq On : 12 Oct 2023 12:14
Operator : MD/SY
Sample : 04792-07DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY1B5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------