

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101223\
 Data File : VU055761.D
 Acq On : 12 Oct 2023 13:05
 Operator : MD/SY
 Sample : 04792-06DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY1B4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055761.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.486	58	61	66	rVB2	6358	5120	0.26%	0.033%
2	1.599	88	96	110	rBV	228303	274226	14.08%	1.774%
3	1.782	141	153	154	rBV3	23945	39770	2.04%	0.257%
4	1.888	179	186	204	rVB	166377	242847	12.47%	1.571%
5	2.502	374	377	378	rBV2	659	378	0.02%	0.002%
6	2.515	378	381	382	rVV2	845	475	0.02%	0.003%
7	2.560	383	395	416	rVV	366170	606771	31.15%	3.924%
8	2.708	439	441	447	rVB4	1215	957	0.05%	0.006%
9	2.785	461	465	472	rVB3	1491	1618	0.08%	0.010%
10	2.872	488	492	495	rBV2	510	478	0.02%	0.003%
11	2.952	516	517	521	rVB2	491	290	0.01%	0.002%
12	3.039	531	544	555	rBV3	5661	11541	0.59%	0.075%
13	3.116	564	568	570	rBV3	1529	1162	0.06%	0.008%
14	3.178	577	587	599	rBV	13869	28884	1.48%	0.187%
15	3.297	620	624	626	rBV2	362	269	0.01%	0.002%
16	3.348	631	640	641	rBV5	3245	3665	0.19%	0.024%
17	3.460	669	675	680	rBV2	406	486	0.02%	0.003%
18	3.628	723	727	733	rBV2	343	328	0.02%	0.002%
19	3.702	744	750	753	rBV2	599	569	0.03%	0.004%
20	3.763	764	769	775	rVB2	383	394	0.02%	0.003%
21	3.869	792	802	808	rBV5	1198	2183	0.11%	0.014%
22	4.071	863	865	871	rVB3	449	418	0.02%	0.003%
23	4.104	871	875	878	rBV	402	371	0.02%	0.002%
24	4.184	897	900	907	rBV2	428	536	0.03%	0.003%
25	4.525	996	1006	1008	rVV3	1143	1233	0.06%	0.008%
26	4.538	1008	1010	1016	rVB5	837	681	0.03%	0.004%
27	4.618	1023	1035	1038	rBV	161859	286982	14.73%	1.856%
28	5.055	1155	1171	1194	rBV	360818	798875	41.01%	5.167%
29	5.332	1253	1257	1266	rVB5	1217	1317	0.07%	0.009%
30	5.374	1266	1270	1273	rBV3	1058	949	0.05%	0.006%
31	5.515	1309	1314	1318	rBV5	1195	1473	0.08%	0.010%
32	5.570	1329	1331	1337	rVB2	429	350	0.02%	0.002%
33	5.718	1353	1377	1409	rBV2	693933	1948021	100.00%	12.599%
34	5.946	1445	1448	1451	rVB2	639	331	0.02%	0.002%
35	6.036	1474	1476	1480	rVB4	589	328	0.02%	0.002%
36	6.161	1513	1515	1519	rVB2	459	270	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101223\
 Data File : VU055761.D
 Acq On : 12 Oct 2023 13:05
 Operator : MD/SY
 Sample : 04792-06DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY1B4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	6.194	1519	1525	1527	rBV2	328	323	0.02%	0.002%
38	6.245	1527	1541	1579	rVV	575120	1114713	57.22%	7.209%
39	6.383	1582	1584	1592	rVV7	2558	2683	0.14%	0.017%
40	6.415	1592	1594	1598	rVV2	419	273	0.01%	0.002%
41	6.444	1600	1603	1605	rVV2	572	277	0.01%	0.002%
42	6.534	1617	1631	1647	rVV6	53690	119427	6.13%	0.772%
43	6.685	1662	1678	1700	rBV	449148	887618	45.57%	5.741%
44	6.859	1730	1732	1737	rVB5	752	617	0.03%	0.004%
45	7.145	1816	1821	1823	rBV2	422	288	0.01%	0.002%
46	7.197	1826	1837	1840	rBV3	3223	5375	0.28%	0.035%
47	7.258	1852	1856	1861	rVB5	880	813	0.04%	0.005%
48	7.341	1879	1882	1885	rBV2	431	275	0.01%	0.002%
49	7.563	1938	1951	1982	rBV	238678	433400	22.25%	2.803%
50	7.698	1987	1993	1995	rBV3	1386	1271	0.07%	0.008%
51	7.894	2041	2054	2077	rBV	850880	1471210	75.52%	9.515%
52	8.078	2109	2111	2114	rVB2	653	295	0.02%	0.002%
53	8.177	2130	2142	2164	rVV	167296	292527	15.02%	1.892%
54	8.345	2191	2194	2198	rVB3	774	513	0.03%	0.003%
55	8.386	2198	2207	2209	rBV3	380	512	0.03%	0.003%
56	8.402	2209	2212	2217	rBV2	638	384	0.02%	0.002%
57	8.457	2225	2229	2232	rBV2	853	575	0.03%	0.004%
58	8.550	2243	2258	2273	rBV	283204	490387	25.17%	3.172%
59	8.634	2273	2284	2329	rVB3	442627	1071005	54.98%	6.927%
60	8.943	2378	2380	2386	rBV2	381	322	0.02%	0.002%
61	9.004	2395	2399	2401	rBV2	553	448	0.02%	0.003%
62	9.049	2411	2413	2419	rVB2	488	393	0.02%	0.003%
63	9.213	2462	2464	2468	rVB2	495	375	0.02%	0.002%
64	9.235	2468	2471	2474	rBV2	609	431	0.02%	0.003%
65	9.415	2514	2527	2556	rBV	845113	1424989	73.15%	9.216%
66	9.611	2585	2588	2591	rVB3	491	292	0.01%	0.002%
67	9.647	2597	2599	2603	rVB	873	466	0.02%	0.003%
68	9.698	2611	2615	2621	rBV3	615	739	0.04%	0.005%
69	10.399	2829	2833	2837	rBV3	477	378	0.02%	0.002%
70	10.502	2857	2865	2867	rBV2	654	923	0.05%	0.006%
71	10.753	2929	2943	2967	rBV	685227	1129576	57.99%	7.305%
72	11.023	3020	3027	3031	rBV	1156	1319	0.07%	0.009%
73	11.148	3064	3066	3071	rVB3	565	321	0.02%	0.002%
74	11.177	3071	3075	3079	rVB2	372	327	0.02%	0.002%
75	11.200	3079	3082	3085	rBV2	507	366	0.02%	0.002%
76	11.248	3093	3097	3103	rVB	599	544	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101223\
 Data File : VU055761.D
 Acq On : 12 Oct 2023 13:05
 Operator : MD/SY
 Sample : 04792-06DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY1B4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	11.290	3103	3110	3111	rBV2	401	393	0.02%	0.003%
78	11.361	3128	3132	3135	rBV	414	307	0.02%	0.002%
79	11.473	3164	3167	3171	rBV3	908	831	0.04%	0.005%
80	11.595	3201	3205	3209	rBV3	419	350	0.02%	0.002%
81	11.650	3220	3222	3229	rVB2	383	357	0.02%	0.002%
82	11.811	3259	3272	3295	rBV	824931	1334474	68.50%	8.631%
83	12.033	3337	3341	3346	rVB4	770	758	0.04%	0.005%
84	12.087	3355	3358	3361	rBV2	431	438	0.02%	0.003%
85	12.190	3377	3390	3412	rBV	835219	1395957	71.66%	9.028%
86	12.367	3442	3445	3448	rBV3	939	549	0.03%	0.004%
87	12.409	3455	3458	3460	rBV3	641	338	0.02%	0.002%
88	12.431	3463	3465	3469	rBV2	448	299	0.02%	0.002%
89	12.553	3500	3503	3509	rBV4	422	483	0.02%	0.003%
90	12.586	3511	3513	3516	rBV2	482	288	0.01%	0.002%
91	12.647	3529	3532	3535	rBV	360	277	0.01%	0.002%
92	12.666	3536	3538	3544	rVB3	471	408	0.02%	0.003%
93	12.952	3624	3627	3630	rVB3	583	297	0.02%	0.002%
94	13.193	3699	3702	3706	rBV3	396	388	0.02%	0.003%
95	13.232	3711	3714	3715	rBV2	503	294	0.02%	0.002%
96	13.274	3724	3727	3732	rBV3	529	445	0.02%	0.003%
97	13.370	3753	3757	3761	rVB3	495	455	0.02%	0.003%
98	13.405	3764	3768	3771	rBV2	427	338	0.02%	0.002%
99	14.627	4145	4148	4152	rBV3	911	884	0.05%	0.006%
100	15.061	4279	4283	4287	rBV2	1331	1089	0.06%	0.007%


Sum of corrected areas: 15462213

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101223\
Data File : VU055761.D
Acq On : 12 Oct 2023 13:05
Operator : MD/SY
Sample : 04792-06DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY1B4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

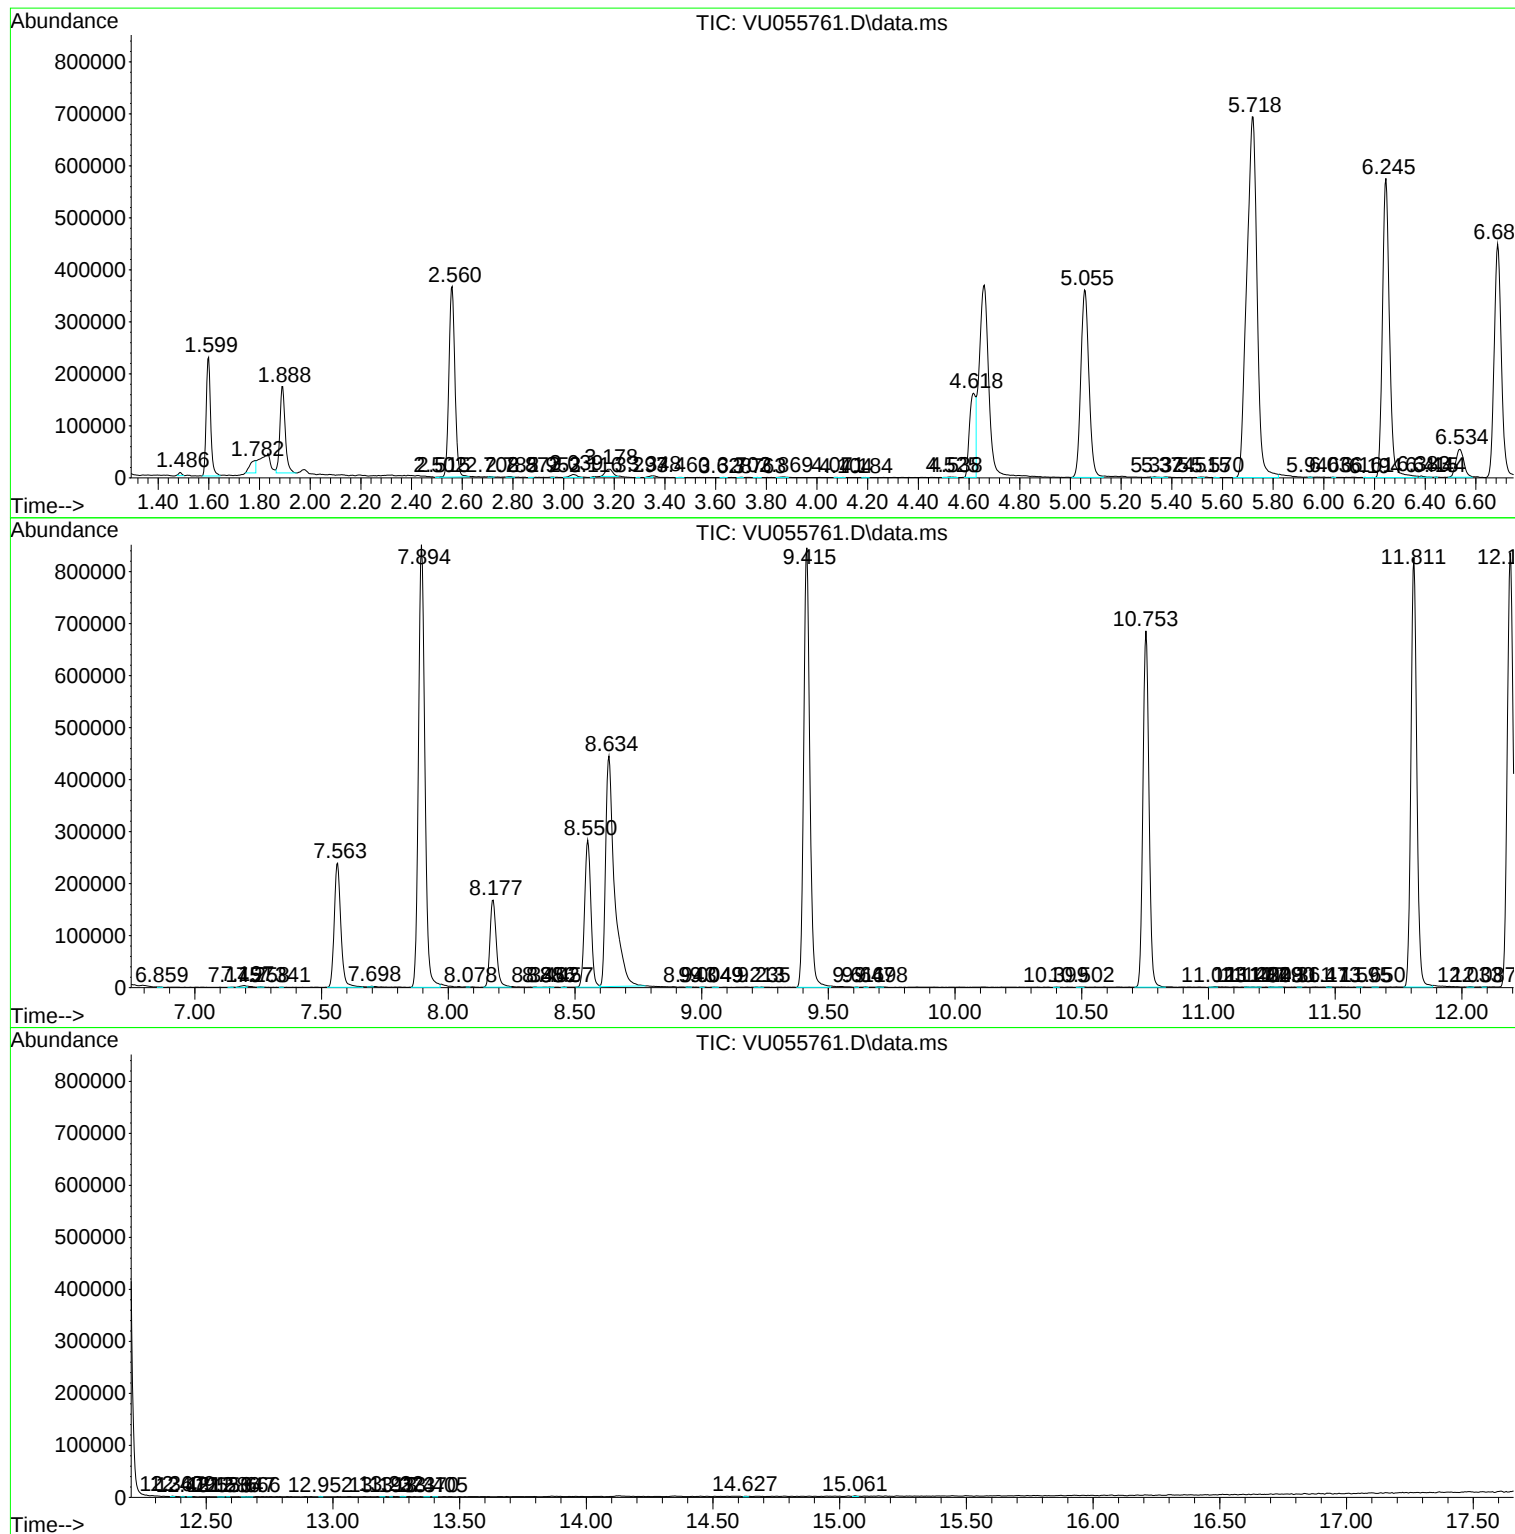

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101223\
Data File : VU055761.D
Acq On : 12 Oct 2023 13:05
Operator : MD/SY
Sample : 04792-06DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY1B4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101223\
Data File : VU055761.D
Acq On : 12 Oct 2023 13:05
Operator : MD/SY
Sample : 04792-06DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY1B4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------