
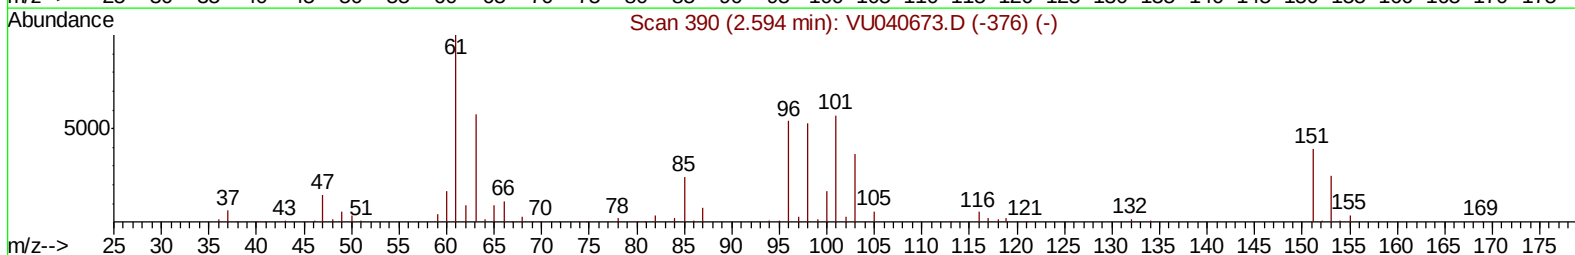
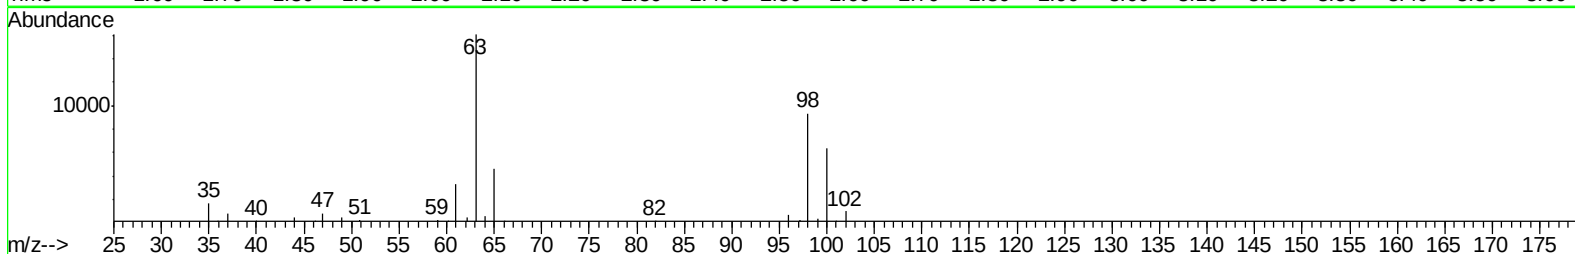


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU101320\
Data File : VU040686.D
Acq On : 13 Oct 2020 16:35
Operator : SY/MD
Sample : L4346-01DL 4X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Oct 14 08:01:18 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Oct 14 05:57:05 2020
Response via : Initial Calibration

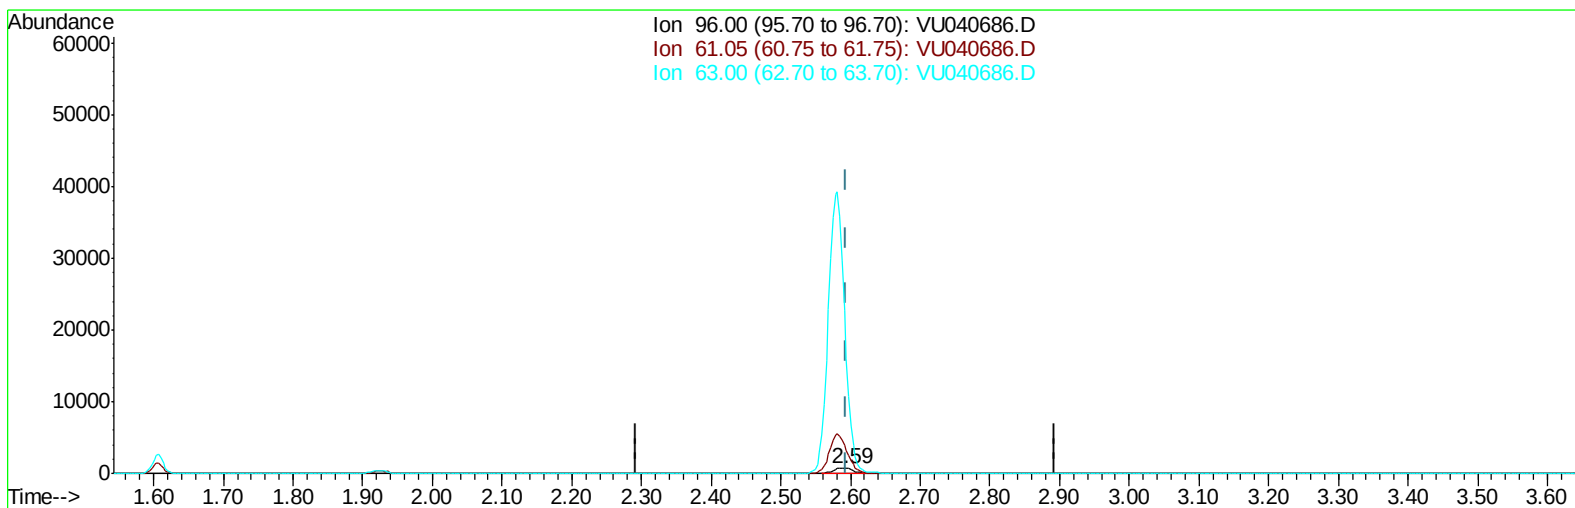

TIC: VU040686.D

(12) 1,1-Dichloroethene (T)

2.594min (+0.000) 0.14ug/L m

response 1313

Ion	Exp%	Act%
96.00	100	100
61.05	184.00	493.08#
63.00	120.90	2418.95#
0.00	0.00	0.00