


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101320\
Data File : VU040686.D
Acq On : 13 Oct 2020 16:35
Operator : SY/MD
Sample : L4346-01DL 4X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YAQZ2DL

Manual Integrations
APPROVED

MMDadoda
10/14/2020 5:14:05 PM

Quant Time: Oct 14 08:02:43 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Oct 14 05:57:05 2020
Response via : Initial Calibration

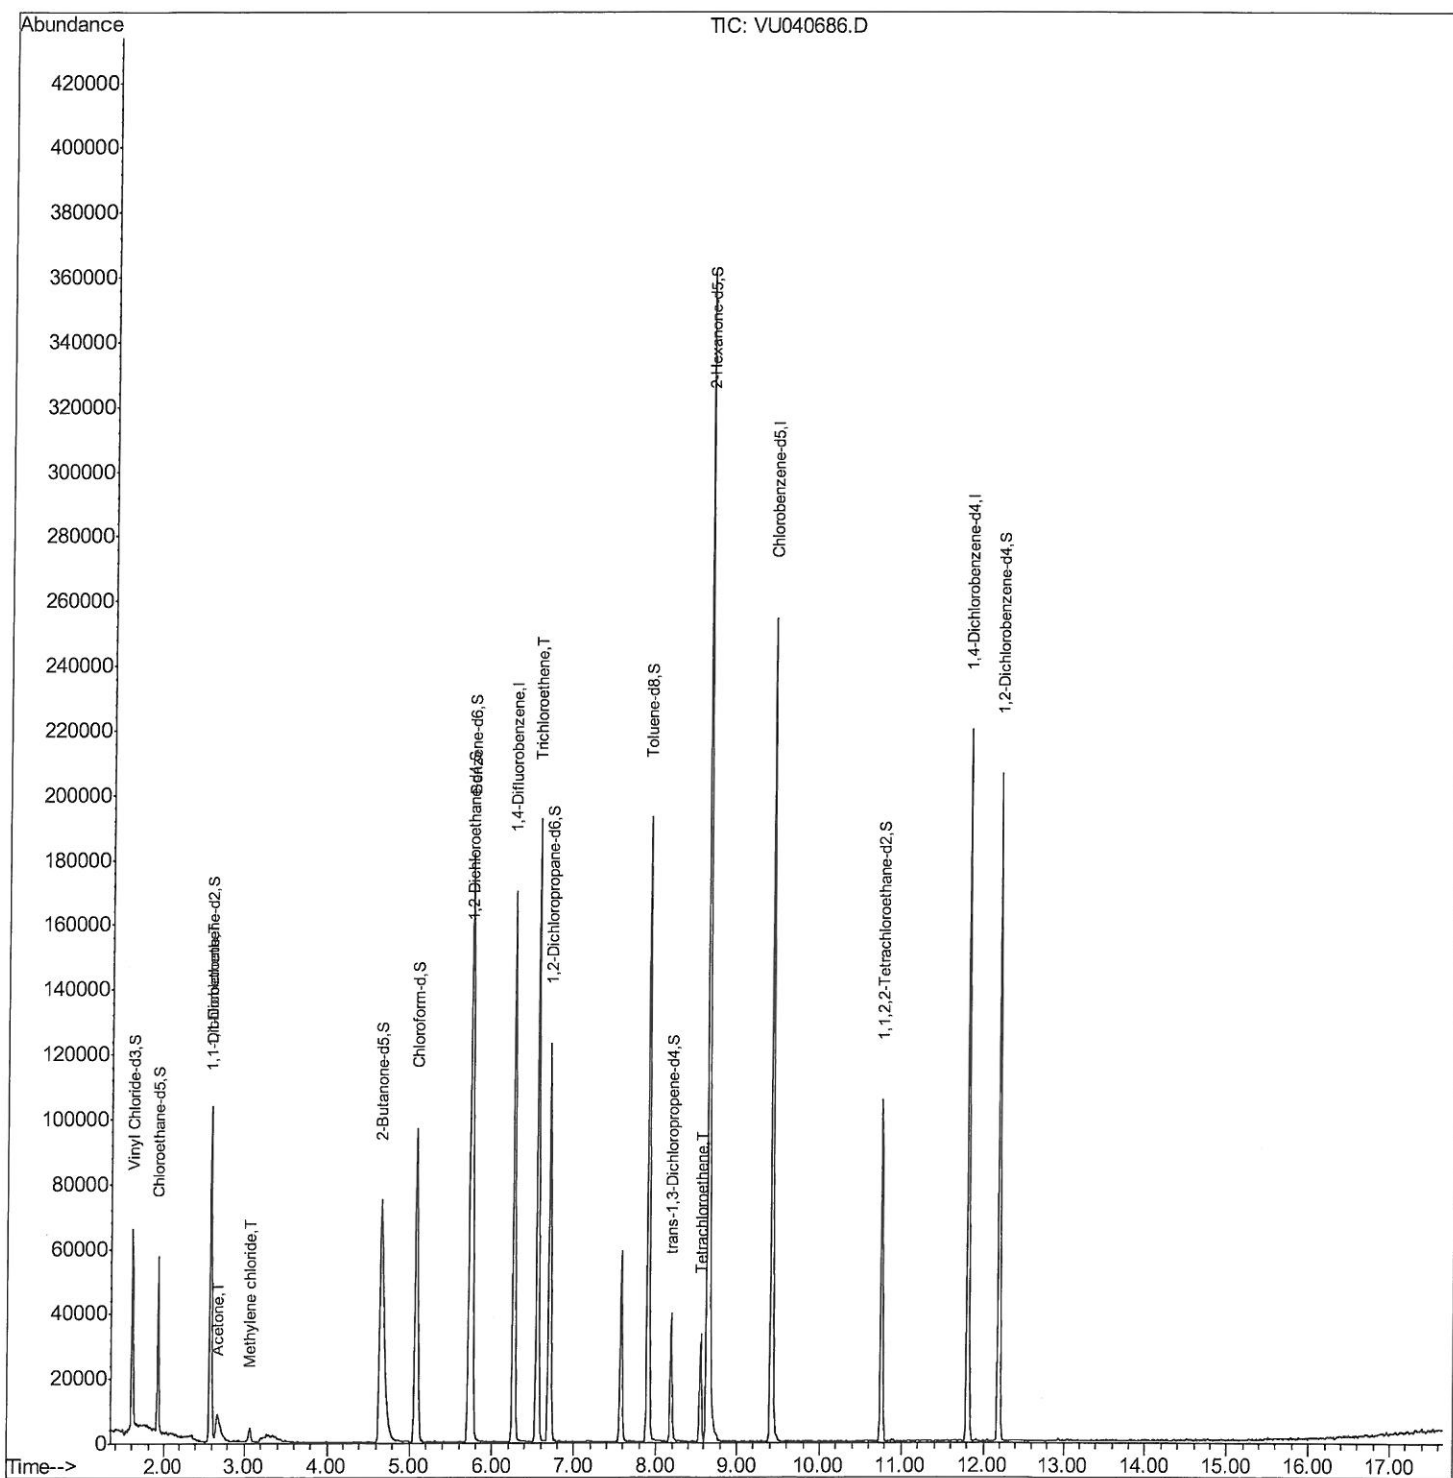

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101320\
 Data File : VU040686.D
 Acq On : 13 Oct 2020 16:35
 Operator : SY/MD
 Sample : L4346-01DL 4X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
ClientSampleId :
 YAQZ2DL

Manual Integrations
APPROVED

MMDadoda
 10/14/2020 5:14:05 PM

Quant Time: Oct 14 08:01:18 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 14 05:57:05 2020
 Response via : Initial Calibration

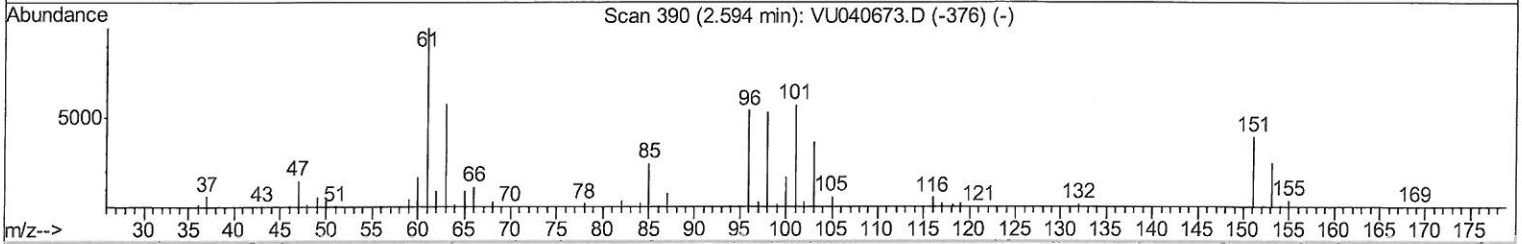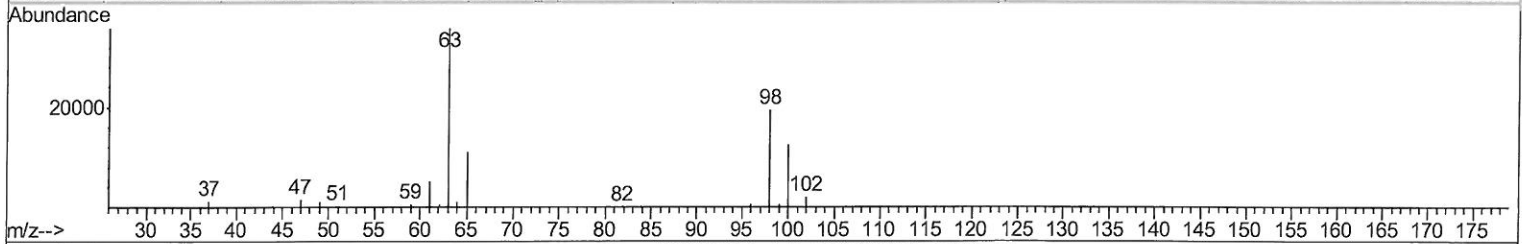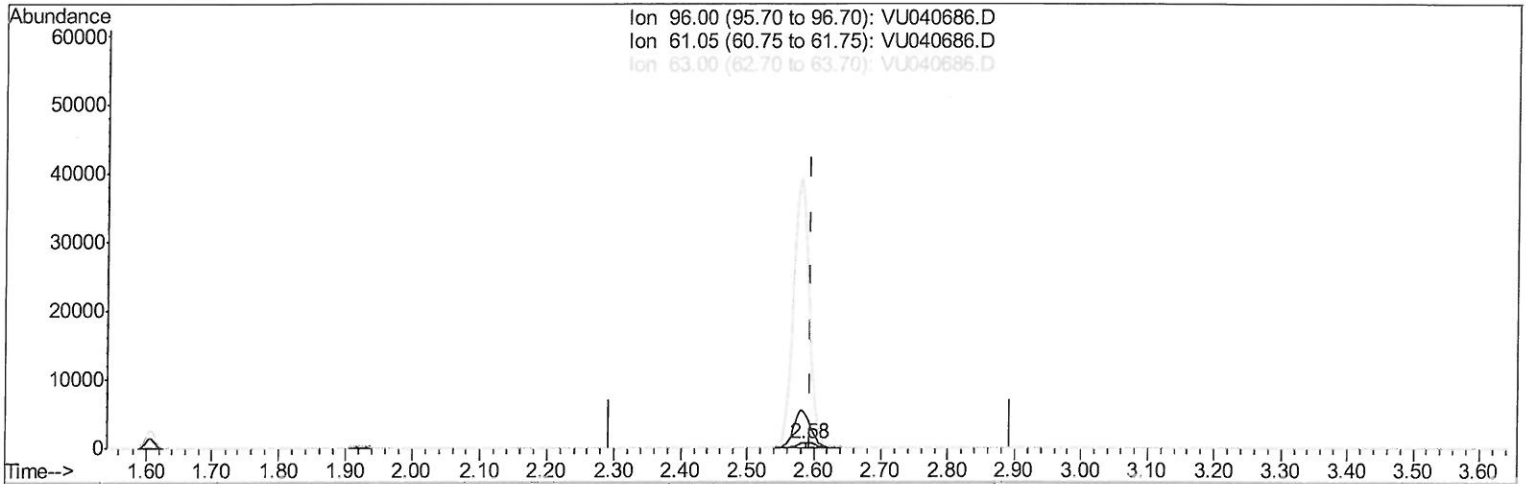

TIC: VU040686.D

(12) 1,1-Dichloroethene (T)

2.585min (-0.009) 0.07ug/L

response 665

Ion	Exp%	Act%
96.00	100	100
61.05	184.00	782.53#
63.00	120.90	5392.77#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101320\
 Data File : VU040686.D
 Acq On : 13 Oct 2020 16:35
 Operator : SY/MD
 Sample : L4346-01DL 4X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YAQZ2DL

Manual Integrations
 APPROVED

MMDadoda
 10/14/2020 5:14:05 PM

Quant Time: Oct 14 08:01:18 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 14 05:57:05 2020
 Response via : Initial Calibration

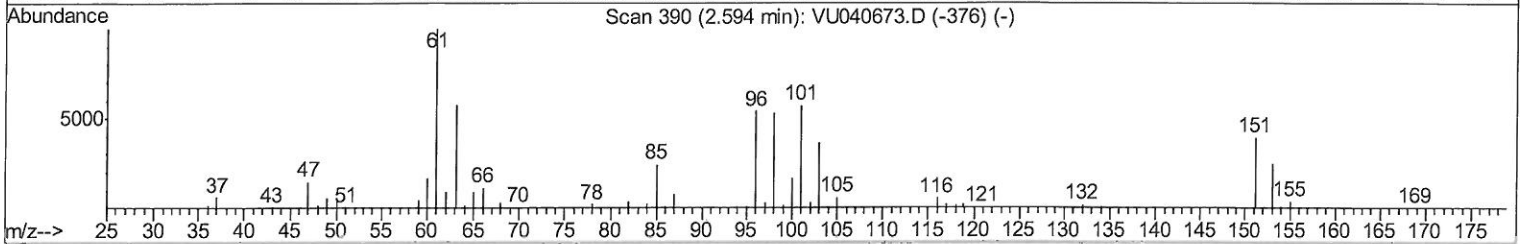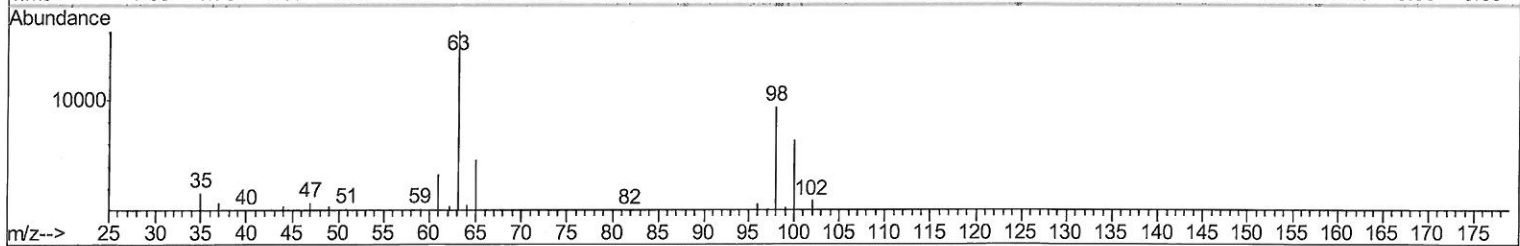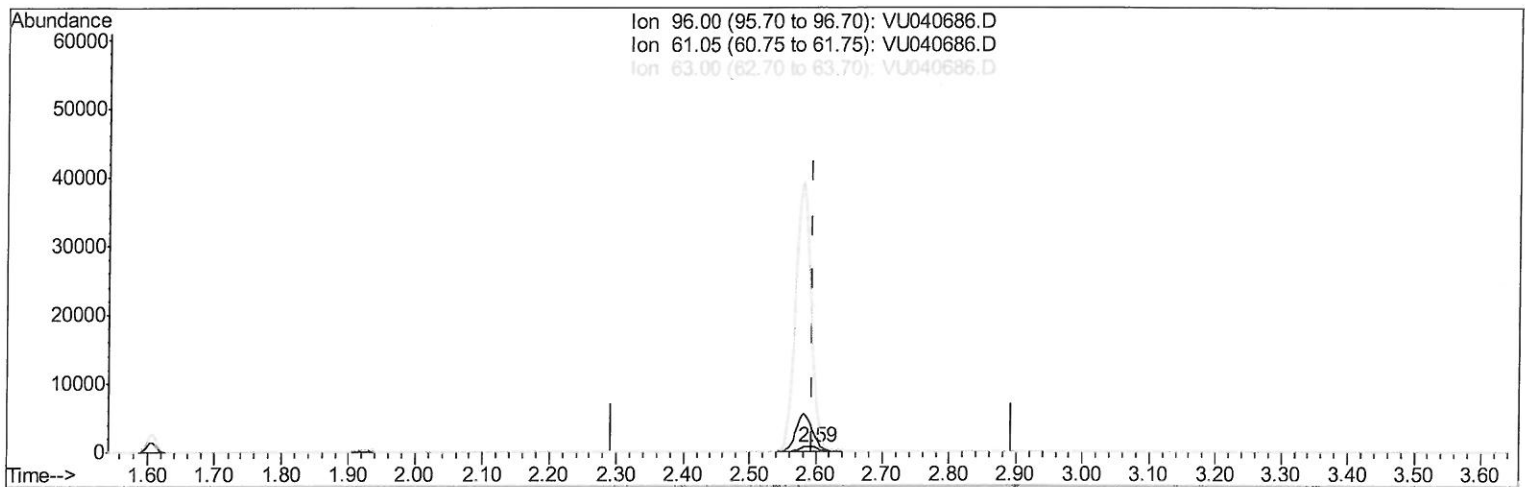

TIC: VU040686.D

(12) 1,1-Dichloroethene (T)

2.594min (+0.000) 0.14ug/L m

response 1313

Ion Exp% Act%

96.00	100	100
61.05	184.00	493.08#
63.00	120.90	2418.95#
0.00	0.00	0.00

Handwritten signature: JMD
 10/15/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101320\
 Data File : VU040686.D
 Acq On : 13 Oct 2020 16:35
 Operator : SY/MD
 Sample : L4346-01DL 4X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YAQZ2DL

Manual Integrations
 APPROVED

MMDadoda
 10/14/2020 5:14:05 PM

Quant Time: Oct 14 08:02:43 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 14 05:57:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	127333	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	131611	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	54693	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	40122	3.80	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.00%
7) Chloroethane-d5	1.92	69	36755	4.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.40%
11) 1,1-Dichloroethene-d2	2.58	63	64484	3.13	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.60%
20) 2-Butanone-d5	4.66	46	177443	52.55	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.10%
24) Chloroform-d	5.08	84	87947	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.00%
26) 1,2-Dichloroethane-d4	5.72	65	54635	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
32) Benzene-d6	5.74	84	152250	4.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.80%
36) 1,2-Dichloropropane-d6	6.70	67	55357	4.70	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.00%
41) Toluene-d8	7.91	98	119579	3.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.20%
43) trans-1,3-Dichloropropene-	8.19	79	21637	4.33	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.60%
46) 2-Hexanone-d5	8.64	63	121832	47.36	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.72%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	50581	4.78	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.60%
64) 1,2-Dichlorobenzene-d4	12.19	152	50544	4.98	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.60%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
12) 1,1-Dichloroethene	2.59	96	1313m	0.145	ug/L	98
13) Acetone	2.67	43	22592	8.632	ug/L	92
16) Methylene chloride	3.06	84	2062	0.177	ug/L	99
34) Trichloroethene	6.56	95	63164	5.763	ug/L	93
47) Tetrachloroethene	8.56	164	6743	0.862	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed