


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU101320\
 Data File : VU040672.D
 Acq On : 13 Oct 2020 10:18
 Operator : SY/MD
 Sample : BFB19
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB19

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Oct 14 05:57:05 2020

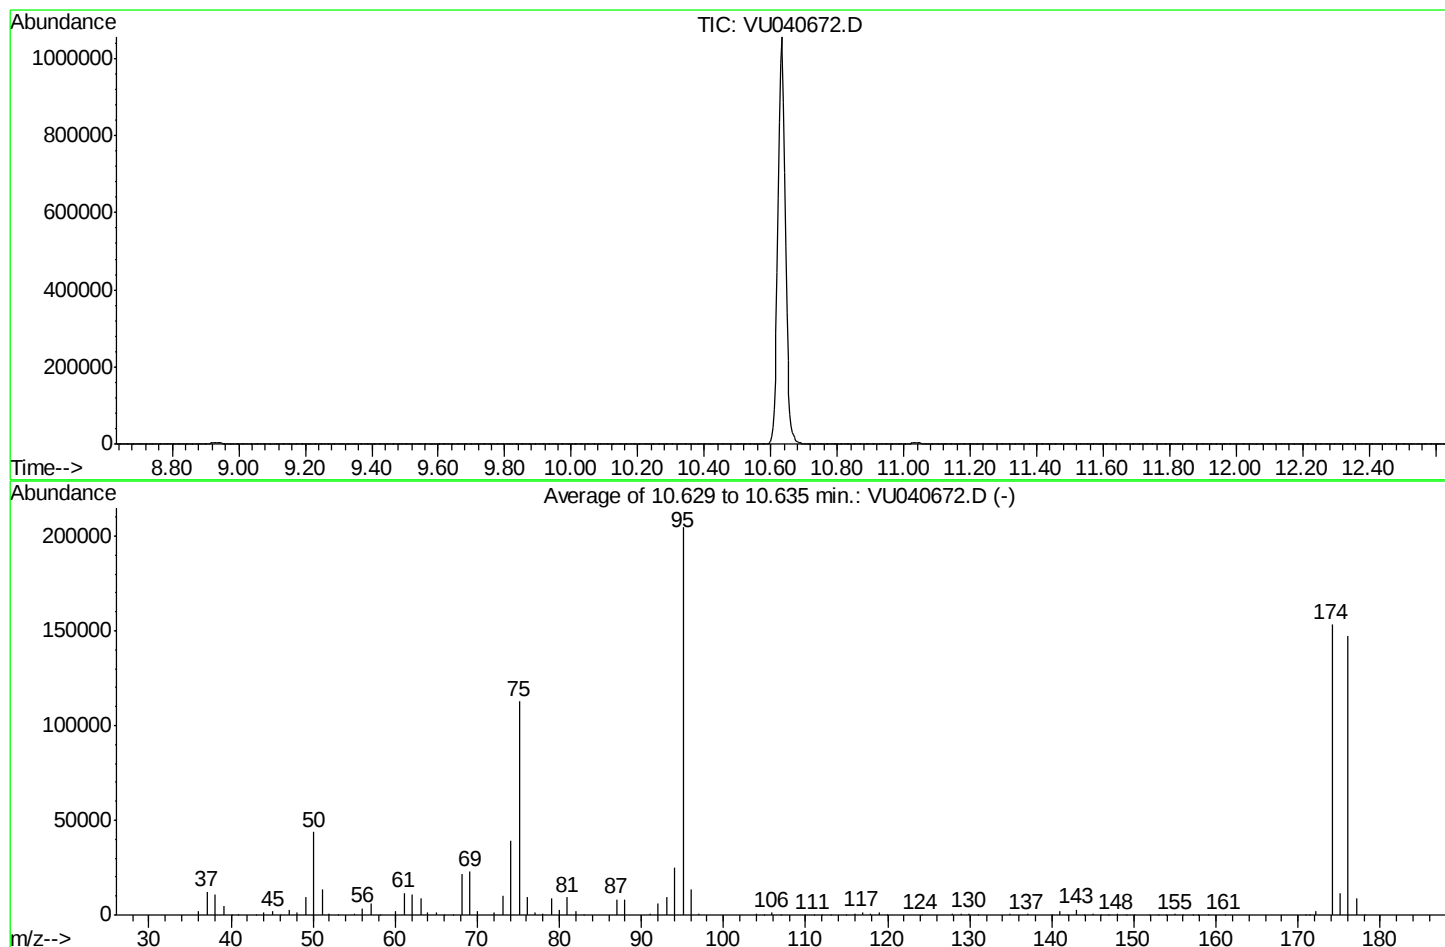

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	43776	PASS
75	95	30	80	55.1	112792	PASS
95	95	100	100	100.0	204565	PASS
96	95	5	9	6.5	13257	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.0	153322	PASS
175	174	5	9	7.5	11498	PASS
176	174	95	101	95.9	147072	PASS
177	176	5	9	6.2	9069	PASS

m/z	Abundance
36.00	2149.0
37.00	12005.0
38.00	10817.0
39.10	4463.0
40.00	343.0
43.10	143.0
44.00	1711.0
45.10	1860.0
46.10	317.0
47.00	2634.0
48.00	1418.0
49.10	9536.0
50.10	43008.0
51.10	13289.0
52.00	676.0
53.00	247.0
55.00	640.0
56.10	3623.0
57.00	6032.0
58.10	421.0
60.00	2337.0
61.10	11246.0
62.10	10988.0
63.10	9319.0
64.00	1287.0
65.10	1642.0
66.00	178.0
67.10	545.0
68.10	21400.0
69.10	22696.0
70.10	1749.0
72.00	1273.0
73.10	9677.0
74.10	37584.0
75.10	110488.0
76.10	9725.0
77.10	1610.0
77.90	864.0
79.00	8676.0
80.00	2570.0
81.00	9310.0
82.00	2086.0
82.90	209.0
87.00	8146.0
88.00	8020.0
91.00	875.0
92.10	5890.0
93.10	9573.0
94.10	24416.0
95.10	198272.0
96.10	12984.0
97.00	380.0
103.90	905.0
104.90	265.0
105.90	1067.0
106.90	192.0
109.90	203.0
111.00	267.0
111.90	186.0
113.00	248.0
114.90	279.0
115.90	1039.0
116.90	1538.0
118.00	1104.0
119.00	1275.0
124.10	109.0
127.90	622.0
128.90	432.0
130.00	677.0
131.00	289.0
134.90	385.0
137.00	380.0
140.00	103.0
141.00	2178.0
141.90	269.0
143.00	2716.0
143.90	287.0
145.00	693.0
145.90	272.0
146.90	133.0
147.90	455.0
149.10	152.0
150.00	228.0
153.90	141.0
155.00	482.0
156.00	228.0
157.00	380.0
159.00	216.0
161.00	272.0
171.10	261.0
172.10	2010.0
174.10	144768.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

175.10	11090.0
176.10	139072.0
177.10	8778.0
178.00	233.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

m/z	Abundance
36.10	2287.0
37.00	12660.0
38.00	11251.0
39.10	4628.0
40.00	369.0
40.80	100.0
43.10	163.0
44.00	1838.0
45.10	2014.0
46.10	308.0
47.10	2601.0
48.00	1483.0
49.10	10036.0
50.10	45232.0
51.10	14014.0
52.00	716.0
53.00	217.0
55.00	696.0
56.00	3715.0
57.00	6624.0
58.10	335.0
60.00	2493.0
61.10	11915.0
62.10	11437.0
63.10	9204.0
64.00	1291.0
65.10	1445.0
66.00	205.0
68.10	22680.0
69.10	23712.0
70.00	1798.0
72.00	1338.0
73.10	10404.0
74.10	40424.0
75.10	116888.0
76.10	10192.0
77.10	1531.0
77.90	877.0
79.00	9093.0
80.00	2791.0
81.00	9489.0
82.00	2190.0
82.90	184.0
87.00	8675.0
88.00	8632.0
91.00	837.0
92.10	6404.0
93.10	10056.0
94.10	26208.0
95.10	211584.0
96.10	13714.0
97.00	378.0
104.00	1072.0
104.90	297.0
105.90	1142.0
106.90	231.0
109.90	217.0
110.90	357.0
112.00	159.0
113.00	215.0
114.90	292.0
116.00	1011.0
117.00	1534.0
117.90	1057.0
119.00	1392.0
124.10	142.0
127.90	751.0
128.90	477.0
129.90	751.0
131.00	321.0
134.90	427.0
137.00	435.0
140.00	146.0
141.00	2208.0
141.90	305.0
143.00	3056.0
143.90	222.0
145.00	630.0
145.90	326.0
147.00	165.0
148.00	516.0
149.00	173.0
150.00	259.0
151.90	110.0
152.90	110.0
153.90	178.0
155.00	505.0
156.00	203.0
157.10	330.0
157.80	109.0
159.10	197.0
161.00	260.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

170.90	240.0
171.30	267.0
172.10	2024.0
174.10	158400.0
175.10	11891.0
176.10	152192.0
177.10	9369.0
178.10	241.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

m/z	Abundance
36.10	2196.0
37.10	11933.0
38.00	10657.0
39.10	4286.0
40.00	385.0
43.10	163.0
44.00	1776.0
45.10	1888.0
46.00	269.0
47.10	2404.0
48.00	1391.0
49.10	9636.0
50.10	43088.0
51.10	13418.0
52.00	657.0
53.00	164.0
55.00	633.0
56.00	3502.0
57.00	6420.0
58.10	235.0
60.00	2303.0
61.10	11449.0
62.00	10833.0
63.10	8507.0
64.00	1234.0
65.00	1292.0
66.00	222.0
68.10	21768.0
69.10	22464.0
70.00	1653.0
72.00	1331.0
73.10	10083.0
74.10	38944.0
75.10	111000.0
76.10	9511.0
77.10	1305.0
78.00	738.0
79.00	8535.0
80.00	2636.0
81.00	8817.0
82.00	2086.0
83.00	164.0
87.00	8180.0
88.00	8198.0
91.00	809.0
92.00	6233.0
93.10	9425.0
94.10	25304.0
95.10	203840.0
96.10	13074.0
97.00	348.0
104.00	1138.0
104.90	324.0
105.90	1050.0
106.90	202.0
109.90	201.0
110.90	361.0
112.00	133.0
113.00	197.0
114.90	300.0
116.00	913.0
117.00	1414.0
117.90	958.0
119.00	1375.0
119.90	101.0
124.10	137.0
127.90	737.0
128.90	397.0
129.90	761.0
131.00	303.0
134.90	403.0
137.10	464.0
139.90	198.0
141.00	2127.0
141.90	304.0
143.00	2982.0
144.00	165.0
145.00	586.0
146.00	349.0
147.00	170.0
148.00	540.0
149.00	159.0
150.00	233.0
152.90	122.0
154.00	163.0
155.00	518.0
156.00	155.0
157.20	257.0
157.80	103.0
159.10	164.0
161.00	190.0
170.90	243.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

172.10	1893.0
174.10	156800.0
175.10	11514.0
176.10	149952.0
177.10	9061.0
178.10	225.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

Scan 2875 (10.584 min): VU040672.D
BFB19

m/z	Abundance
40.00	167.0
44.00	375.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19