

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101321\
 Data File : VU045306.D
 Acq On : 13 Oct 2021 13:57
 Operator : SY/MD
 Sample : VU1013WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1013WBL01

Quant Time: Oct 14 06:16:14 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101321DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Oct 14 05:46:27 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Fluorobenzene	6.121	96	39265	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.639	95	13181	0.914	ug/l	0.00
Spiked Amount 1.000			Recovery	=	91.000%	
68) 1,2-Dichlorobenzene-d4	12.201	152	12361	0.916	ug/l	0.00
Spiked Amount 1.000			Recovery	=	92.000%	
Target Compounds						
15) Methylene Chloride	3.051	84	4898	0.396	ug/l	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101321\
Data File : VU045306.D
Acq On : 13 Oct 2021 13:57
Operator : SY/MD
Sample : VU1013WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1013WBL01

Quant Time: Oct 14 06:16:14 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101321DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Oct 14 05:46:27 2021
Response via : Initial Calibration




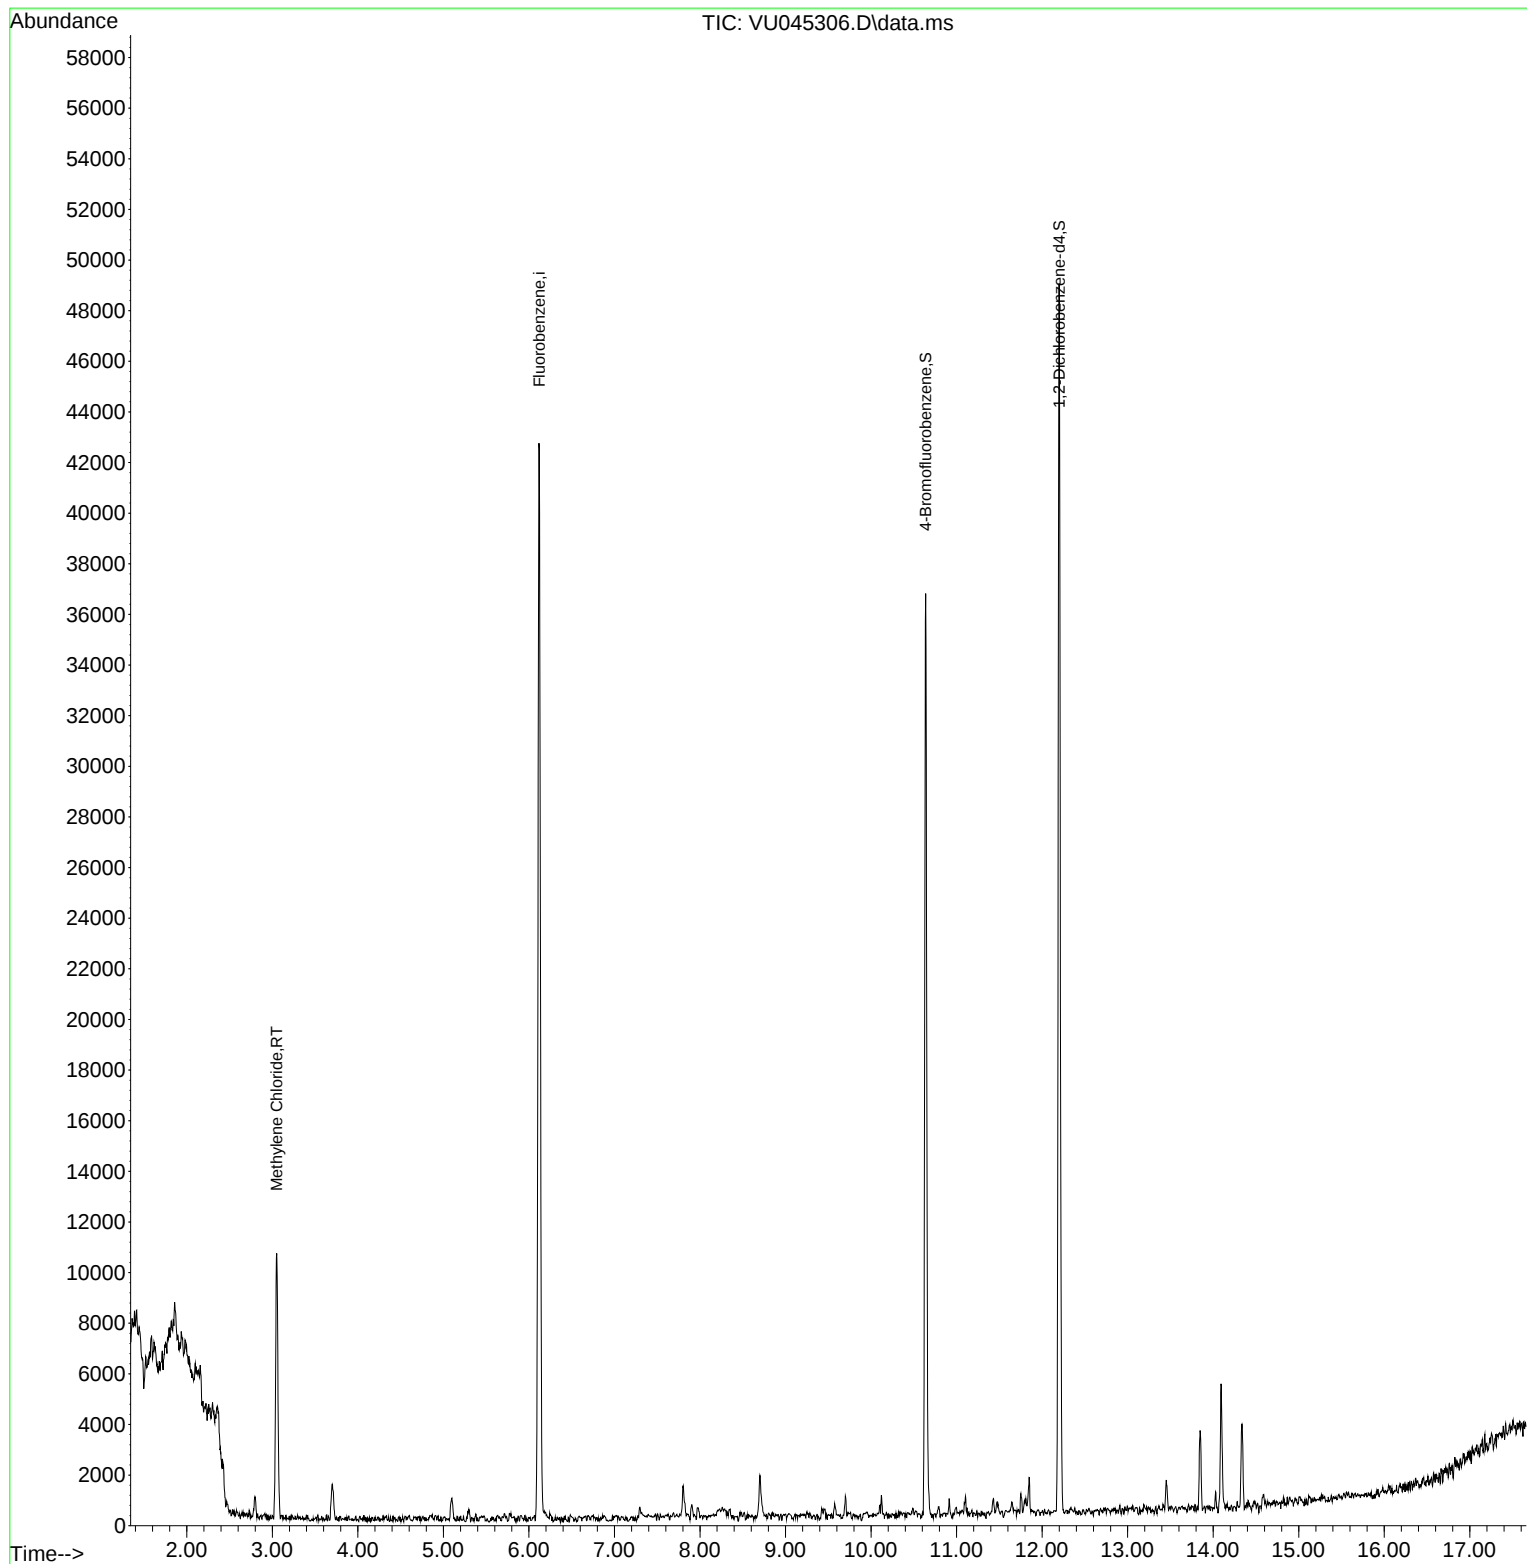


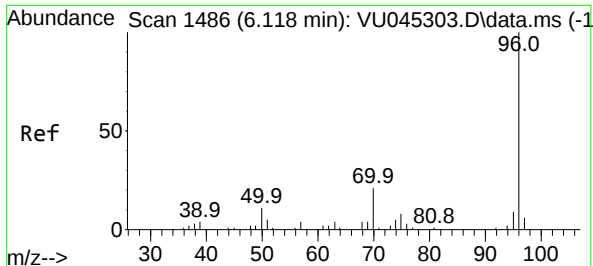

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.121 min Scan# 1487
Delta R.T. 0.003 min
Lab File: VU045306.D
Acq: 13 Oct 2021 13:57




Instrument :
MSVOA_U
ClientSampleId :
VU1013WBL01


Tgt Ion: 96	Resp: 39265
Ion Ratio	Lower Upper
96 100	
70 21.4	16.8 25.2
95 9.2	7.3 10.9
97 6.5	0.0 0.0#

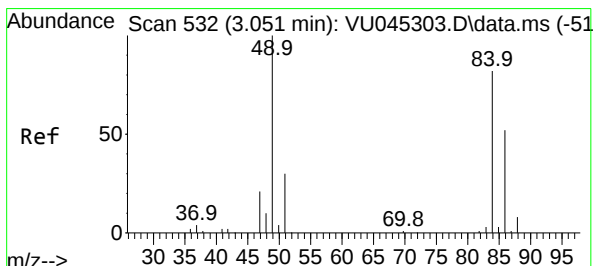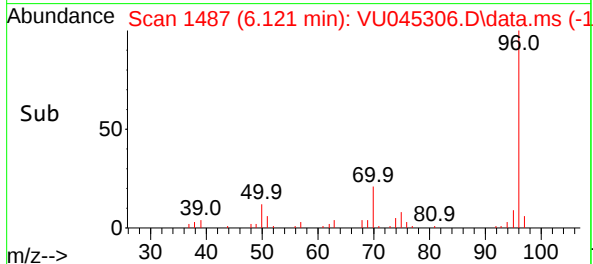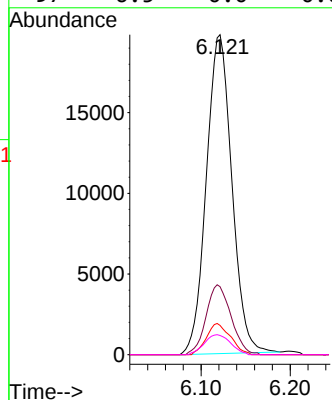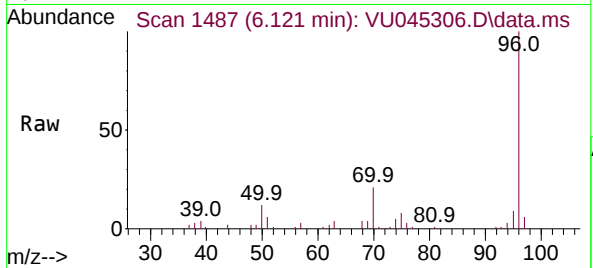

#15
Methylene Chloride
Concen: 0.396 ug/l
RT: 3.051 min Scan# 532
Delta R.T. 0.000 min
Lab File: VU045306.D
Acq: 13 Oct 2021 13:57

Tgt Ion: 84	Resp: 4898
Ion Ratio	Lower Upper
84 100	
49 135.5	97.2 145.8
51 45.6	0.0 73.4
86 72.3	50.2 75.4


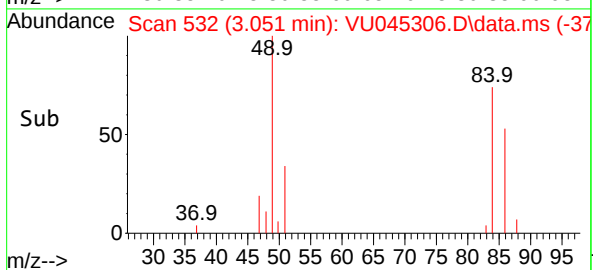
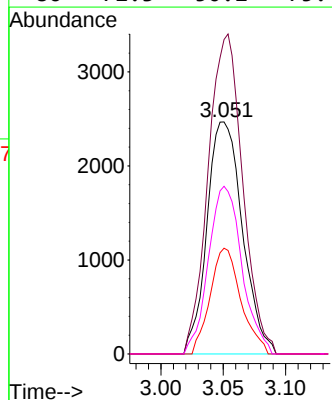
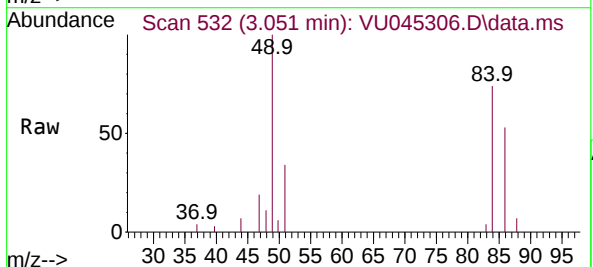


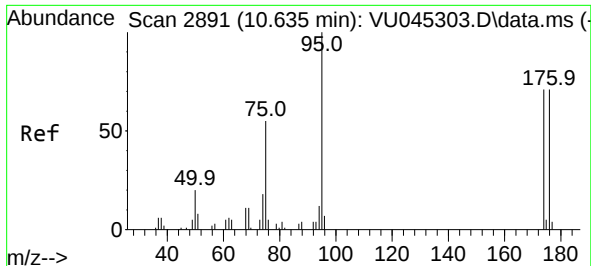

#57
4-Bromofluorobenzene
Concen: 0.914 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. 0.003 min
Lab File: VU045306.D
Acq: 13 Oct 2021 13:57

Instrument :
MSVOA_U
ClientSampleId :
VU1013WBL01

Tgt Ion: 95 Resp: 13181
Ion Ratio Lower Upper
95 100
174 70.4 56.6 84.8
176 67.3 54.3 81.5

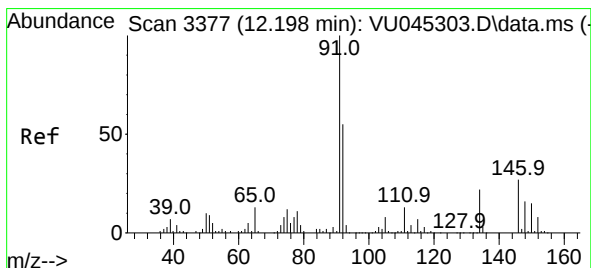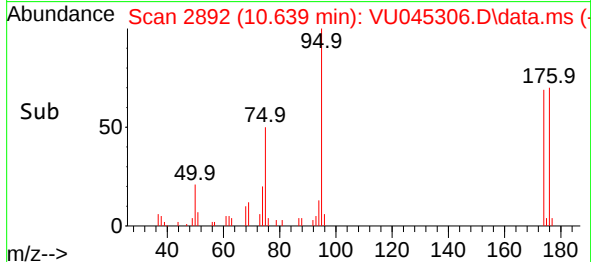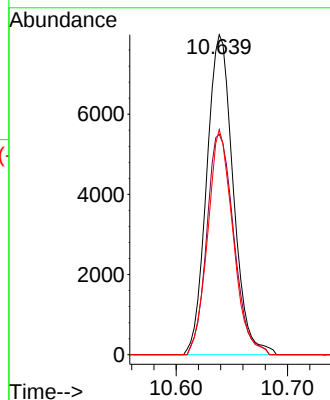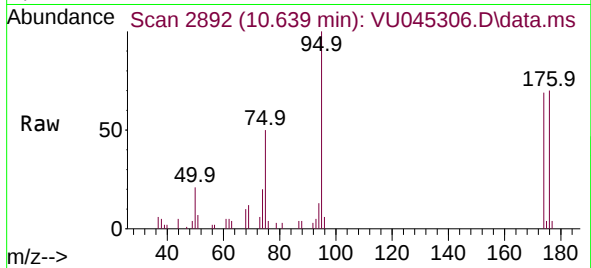

#68
1,2-Dichlorobenzene-d4
Concen: 0.916 ug/l
RT: 12.201 min Scan# 3378
Delta R.T. 0.003 min
Lab File: VU045306.D
Acq: 13 Oct 2021 13:57

Tgt Ion: 152 Resp: 12361
Ion Ratio Lower Upper
152 100
115 65.3 0.0 251.0
150 154.3 0.0 613.8

