

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101321\
 Data File : VU045306.D
 Acq On : 13 Oct 2021 13:57
 Operator : SY/MD
 Sample : VU1013WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1013WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101321DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU045306.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.797	445	453	460	rVB2	847	1313	1.57%	0.470%
2	3.051	521	532	545	rBV2	10491	19691	23.48%	7.043%
3	3.700	725	734	747	rBV6	1414	2815	3.36%	1.007%
4	5.099	1160	1169	1176	rBV2	883	1624	1.94%	0.581%
5	6.118	1472	1486	1505	rBV	42568	83869	100.00%	29.997%
6	7.806	2002	2011	2016	rBV4	1150	1719	2.05%	0.615%
7	7.903	2035	2041	2048	rBV3	609	971	1.16%	0.347%
8	8.700	2277	2289	2304	rBV3	1688	3385	4.04%	1.211%
9	9.700	2594	2600	2606	rVB	796	843	1.01%	0.302%
10	10.639	2882	2892	2910	rBV	36412	58379	69.61%	20.880%
11	10.915	2972	2978	2988	rVB2	775	934	1.11%	0.334%
12	11.475	3144	3152	3163	rVB3	490	874	1.04%	0.313%
13	11.751	3234	3238	3244	rBV3	784	884	1.05%	0.316%
14	11.848	3261	3268	3274	rVB4	1369	1704	2.03%	0.609%
15	12.198	3366	3377	3391	rBV	48507	80518	96.00%	28.799%
16	13.452	3761	3767	3775	rVB3	1200	1643	1.96%	0.588%
17	13.848	3882	3890	3898	rVB4	3151	4769	5.69%	1.706%
18	14.092	3955	3966	3980	rBV	5111	8286	9.88%	2.964%
19	14.336	4034	4042	4050	rVB6	3384	5367	6.40%	1.920%




Sum of corrected areas: 279588

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101321\
Data File : VU045306.D
Acq On : 13 Oct 2021 13:57
Operator : SY/MD
Sample : VU1013WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1013WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101321DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

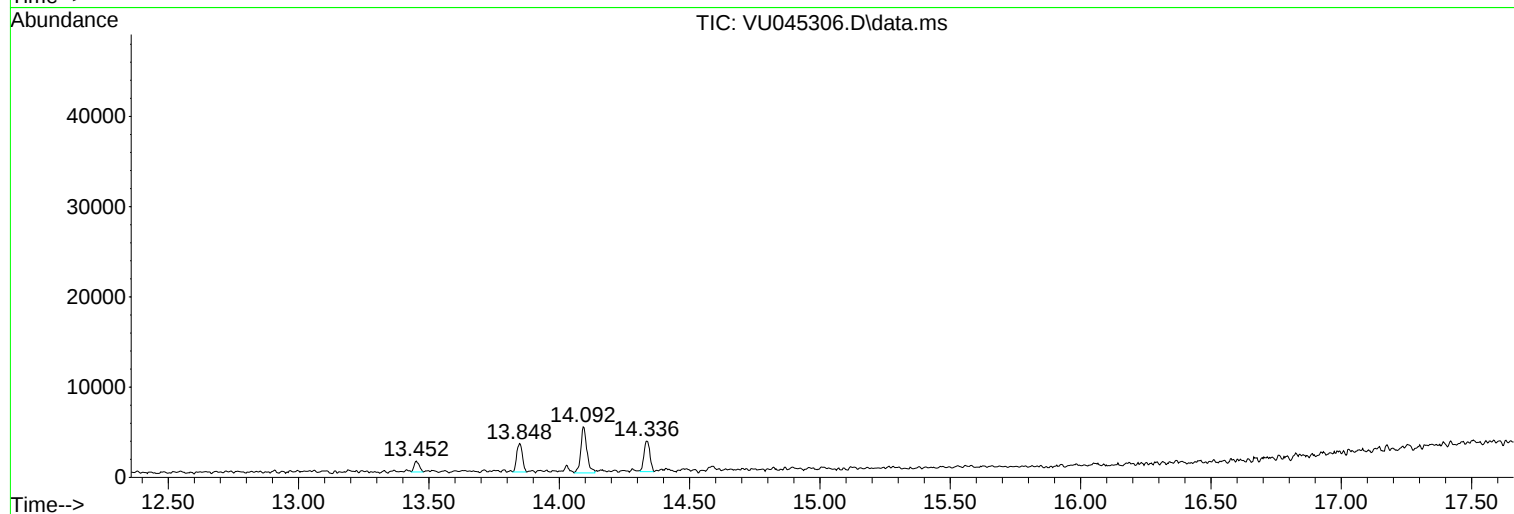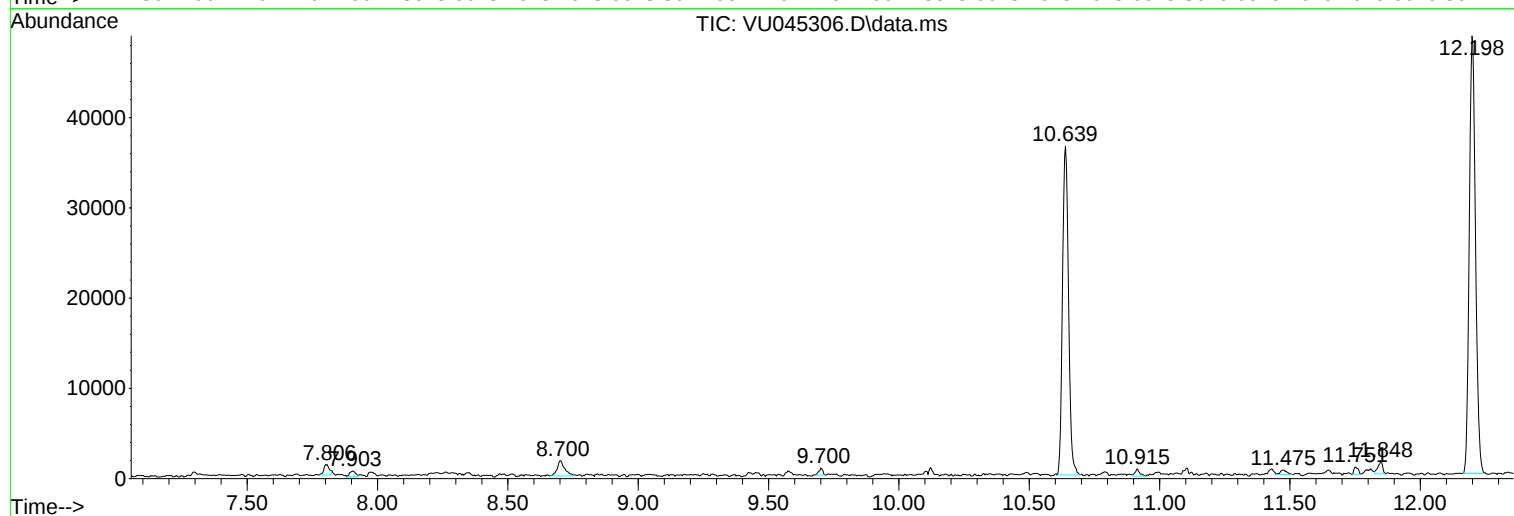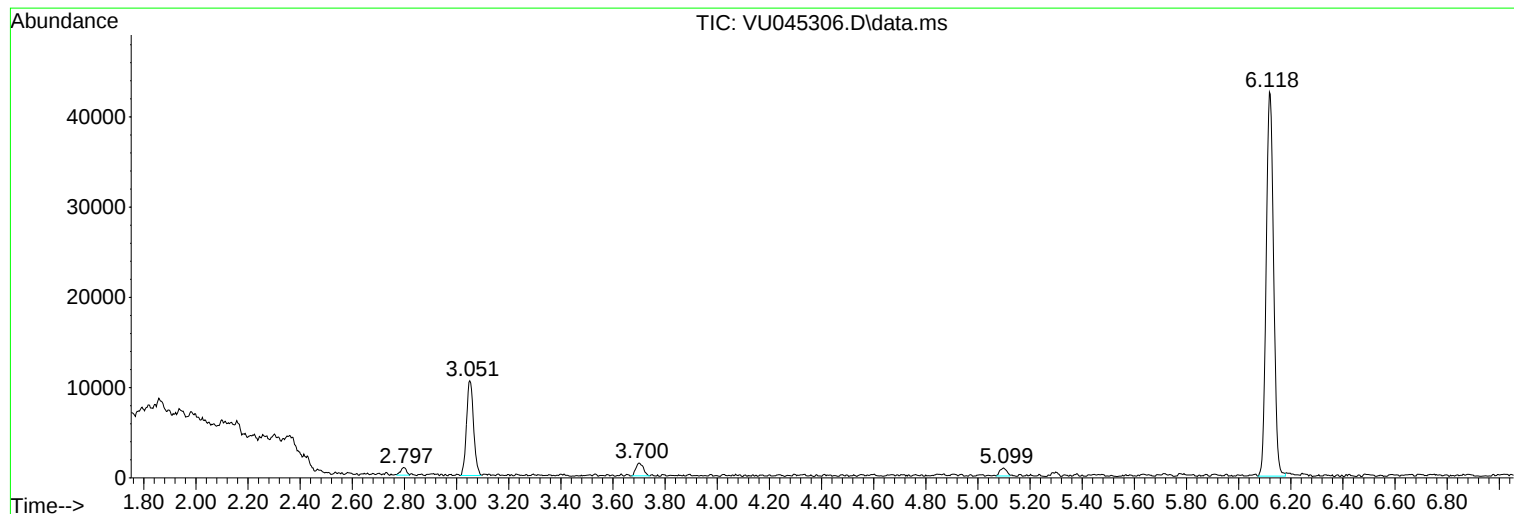

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101321\
Data File : VU045306.D
Acq On : 13 Oct 2021 13:57
Operator : SY/MD
Sample : VU1013WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1013WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101321DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101321\
Data File : VU045306.D
Acq On : 13 Oct 2021 13:57
Operator : SY/MD
Sample : VU1013WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1013WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101321DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------