


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101321\
Data File : VU045298.D
Acq On : 13 Oct 2021 09:05
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101321DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Thu Oct 14 05:46:27 2021

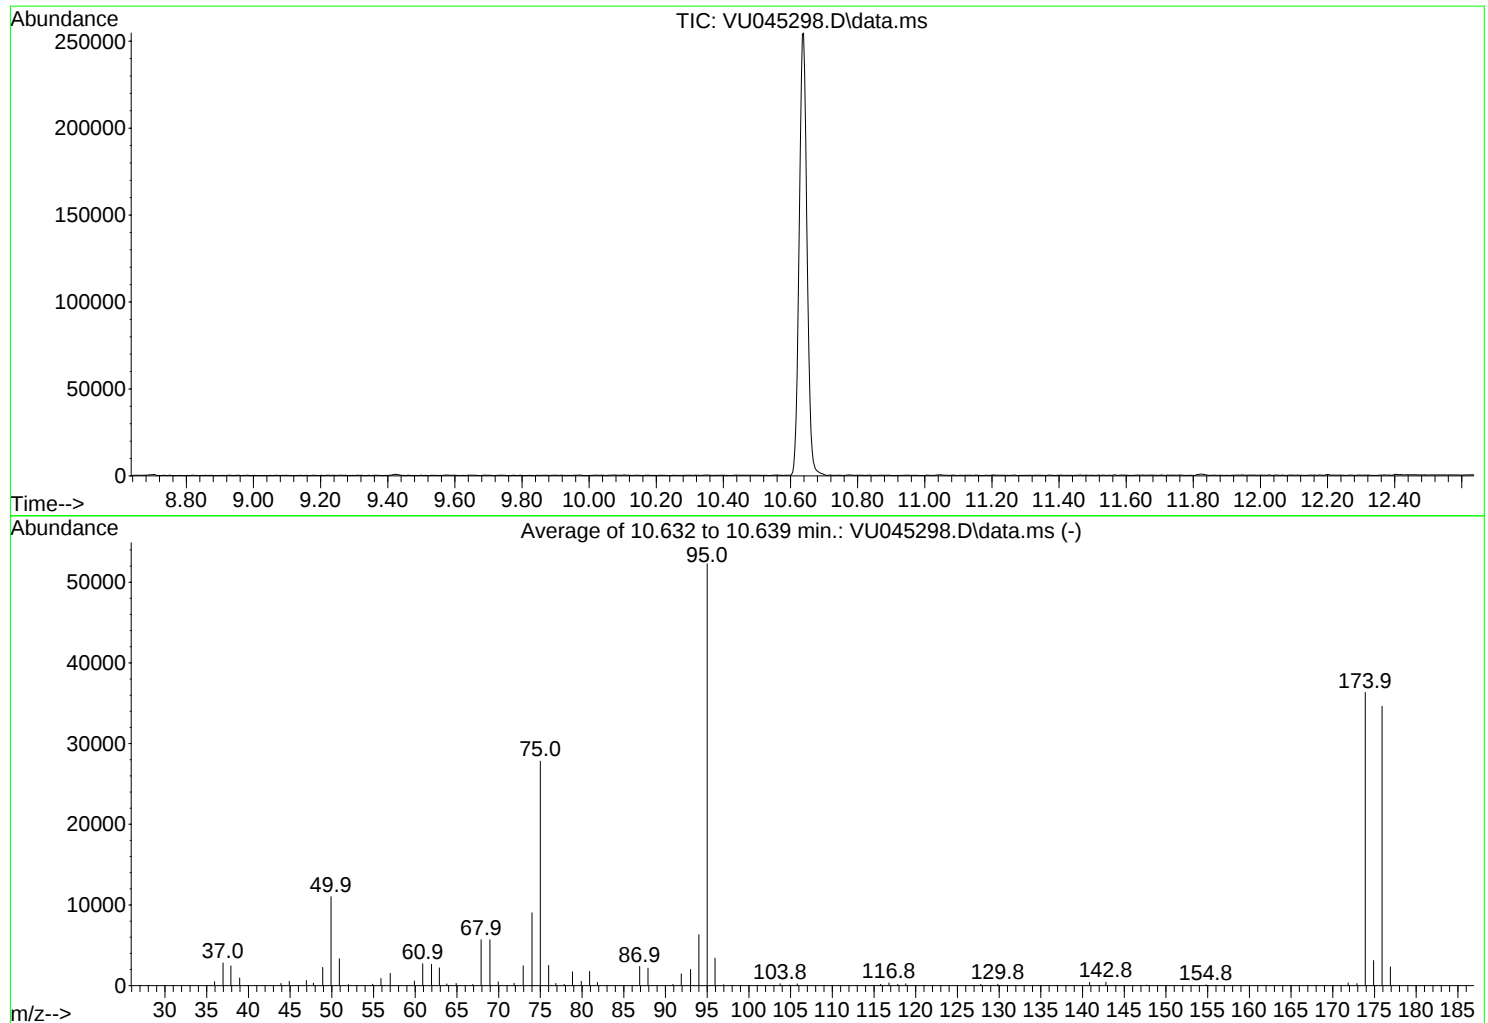

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	11036	PASS
75	95	30	60	53.2	27819	PASS
95	95	100	100	100.0	52277	PASS
96	95	5	9	6.5	3402	PASS
173	174	0.00	2	0.7	252	PASS
174	95	50	100	69.5	36341	PASS
175	174	5	9	8.6	3111	PASS
176	174	95	101	95.3	34635	PASS
177	176	5	9	6.7	2316	PASS