

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101322\
 Data File : VU051406.D
 Acq On : 13 Oct 2022 13:27
 Operator : JC/MD
 Sample : VU1013WBL02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK117

Quant Time: Oct 14 01:21:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 14 01:20:41 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	183880	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	202096	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	69408	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	94409	6.365	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 127.400%		
7) Chloroethane-d5	1.909	69	74826	5.871	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 117.400%		
11) 1,1-Dichloroethene-d2	2.562	65	30309	5.169	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 103.400%		
20) 2-Butanone-d5	4.639	46	158424	48.512	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 97.020%		
24) Chloroform-d	5.063	84	153750	5.560	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 111.200%		
26) 1,2-Dichloroethane-d4	5.703	65	78849	5.529	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 110.600%		
32) Benzene-d6	5.726	84	274474	4.937	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 98.800%		
36) 1,2-Dichloropropane-d6	6.690	67	99254	5.257	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 105.200%		
41) Toluene-d8	7.896	98	199574	4.012	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 80.200%		
43) trans-1,3-Dichloroprop...	8.179	79	29142	4.698	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 94.000%		
46) 2-Hexanone-d5	8.636	63	88353	42.260	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 84.520%		
56) 1,1,2,2-Tetrachloroeth...	10.755	84	73636	4.882	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 97.600%		
66) 1,2-Dichlorobenzene-d4	12.192	152	62934	5.217	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 104.400%		
Target Compounds						
16) Methylene chloride	3.044	84	12418	0.627	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101322\
Data File : VU051406.D
Acq On : 13 Oct 2022 13:27
Operator : JC/MD
Sample : VU1013WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK117

Quant Time: Oct 14 01:21:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 14 01:20:41 2022
Response via : Initial Calibration

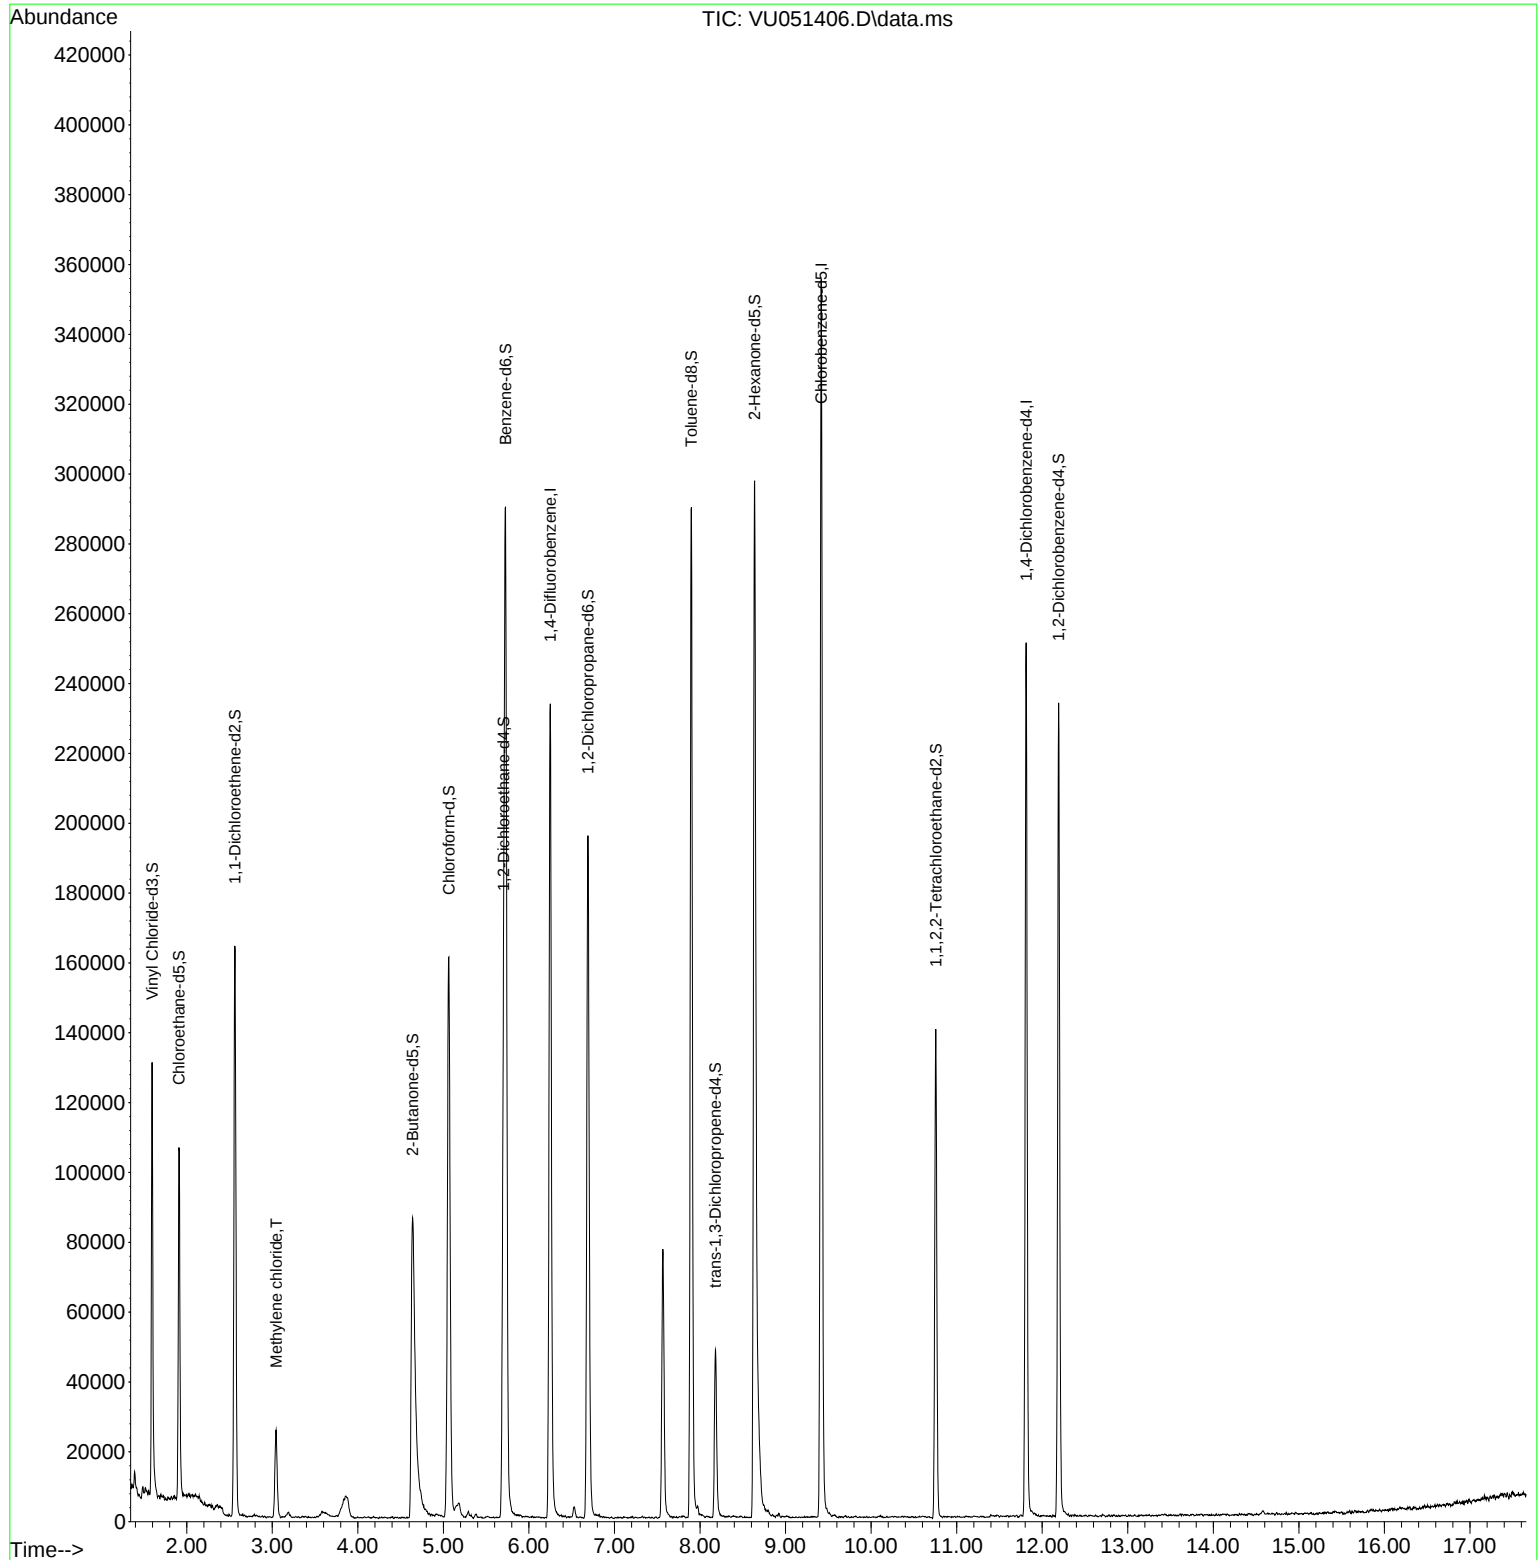

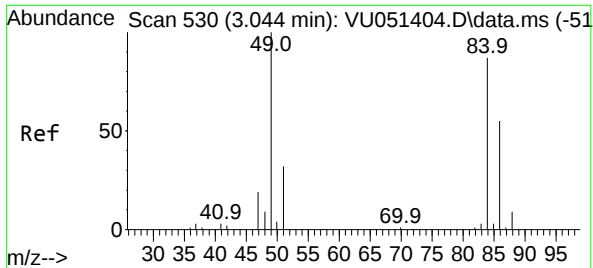

#16
Methylene chloride
Concen: 0.627 ug/L
RT: 3.044 min Scan# 51
Delta R.T. -0.000 min
Lab File: VU051406.D
Acq: 13 Oct 2022 13:27

Instrument :
MSVOA_U
ClientSampleId :
VBLK117

Tgt Ion:	84	Resp:	12418
Ion	Ratio	Lower	Upper
84	100		
86	63.0	46.5	86.3
49	106.9	81.3	151.1

