

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101322\
 Data File : VU051411.D
 Acq On : 13 Oct 2022 16:43
 Operator : JC/MD
 Sample : N4899-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Oct 14 01:22:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 14 01:20:41 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		6.250	114	173432	5.000	ug/L	0.00
28) Chlorobenzene-d5		9.417	117	191867	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.813	152	65236	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.594	65	82809	5.919	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130		Recovery	=	118.400%	
7) Chloroethane-d5		1.909	69	67444	5.611	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130		Recovery	=	112.200%	
11) 1,1-Dichloroethene-d2		2.562	65	30355	5.489	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125		Recovery	=	109.800%	
20) 2-Butanone-d5		4.639	46	178715	58.023	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130		Recovery	=	116.040%	
24) Chloroform-d		5.060	84	144653	5.546	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125		Recovery	=	111.000%	
26) 1,2-Dichloroethane-d4		5.700	65	76813	5.711	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130		Recovery	=	114.200%	
32) Benzene-d6		5.726	84	252617	4.786	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125		Recovery	=	95.800%	
36) 1,2-Dichloropropane-d6		6.687	67	91694	5.115	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140		Recovery	=	102.400%	
41) Toluene-d8		7.896	98	179897	3.810	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130		Recovery	=	76.200%	
43) trans-1,3-Dichloroprop...		8.179	79	28196	4.788	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130		Recovery	=	95.800%	
46) 2-Hexanone-d5		8.633	63	100673	50.720	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130		Recovery	=	101.440%	
56) 1,1,2,2-Tetrachloroeth...		10.755	84	77641	5.422	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120		Recovery	=	108.400%	
66) 1,2-Dichlorobenzene-d4		12.192	152	59064	5.209	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120		Recovery	=	104.200%	
Target Compounds							
16) Methylene chloride		3.041	84	14815	0.793	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101322\
Data File : VU051411.D
Acq On : 13 Oct 2022 16:43
Operator : JC/MD
Sample : N4899-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001


Quant Time: Oct 14 01:22:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 14 01:20:41 2022
Response via : Initial Calibration

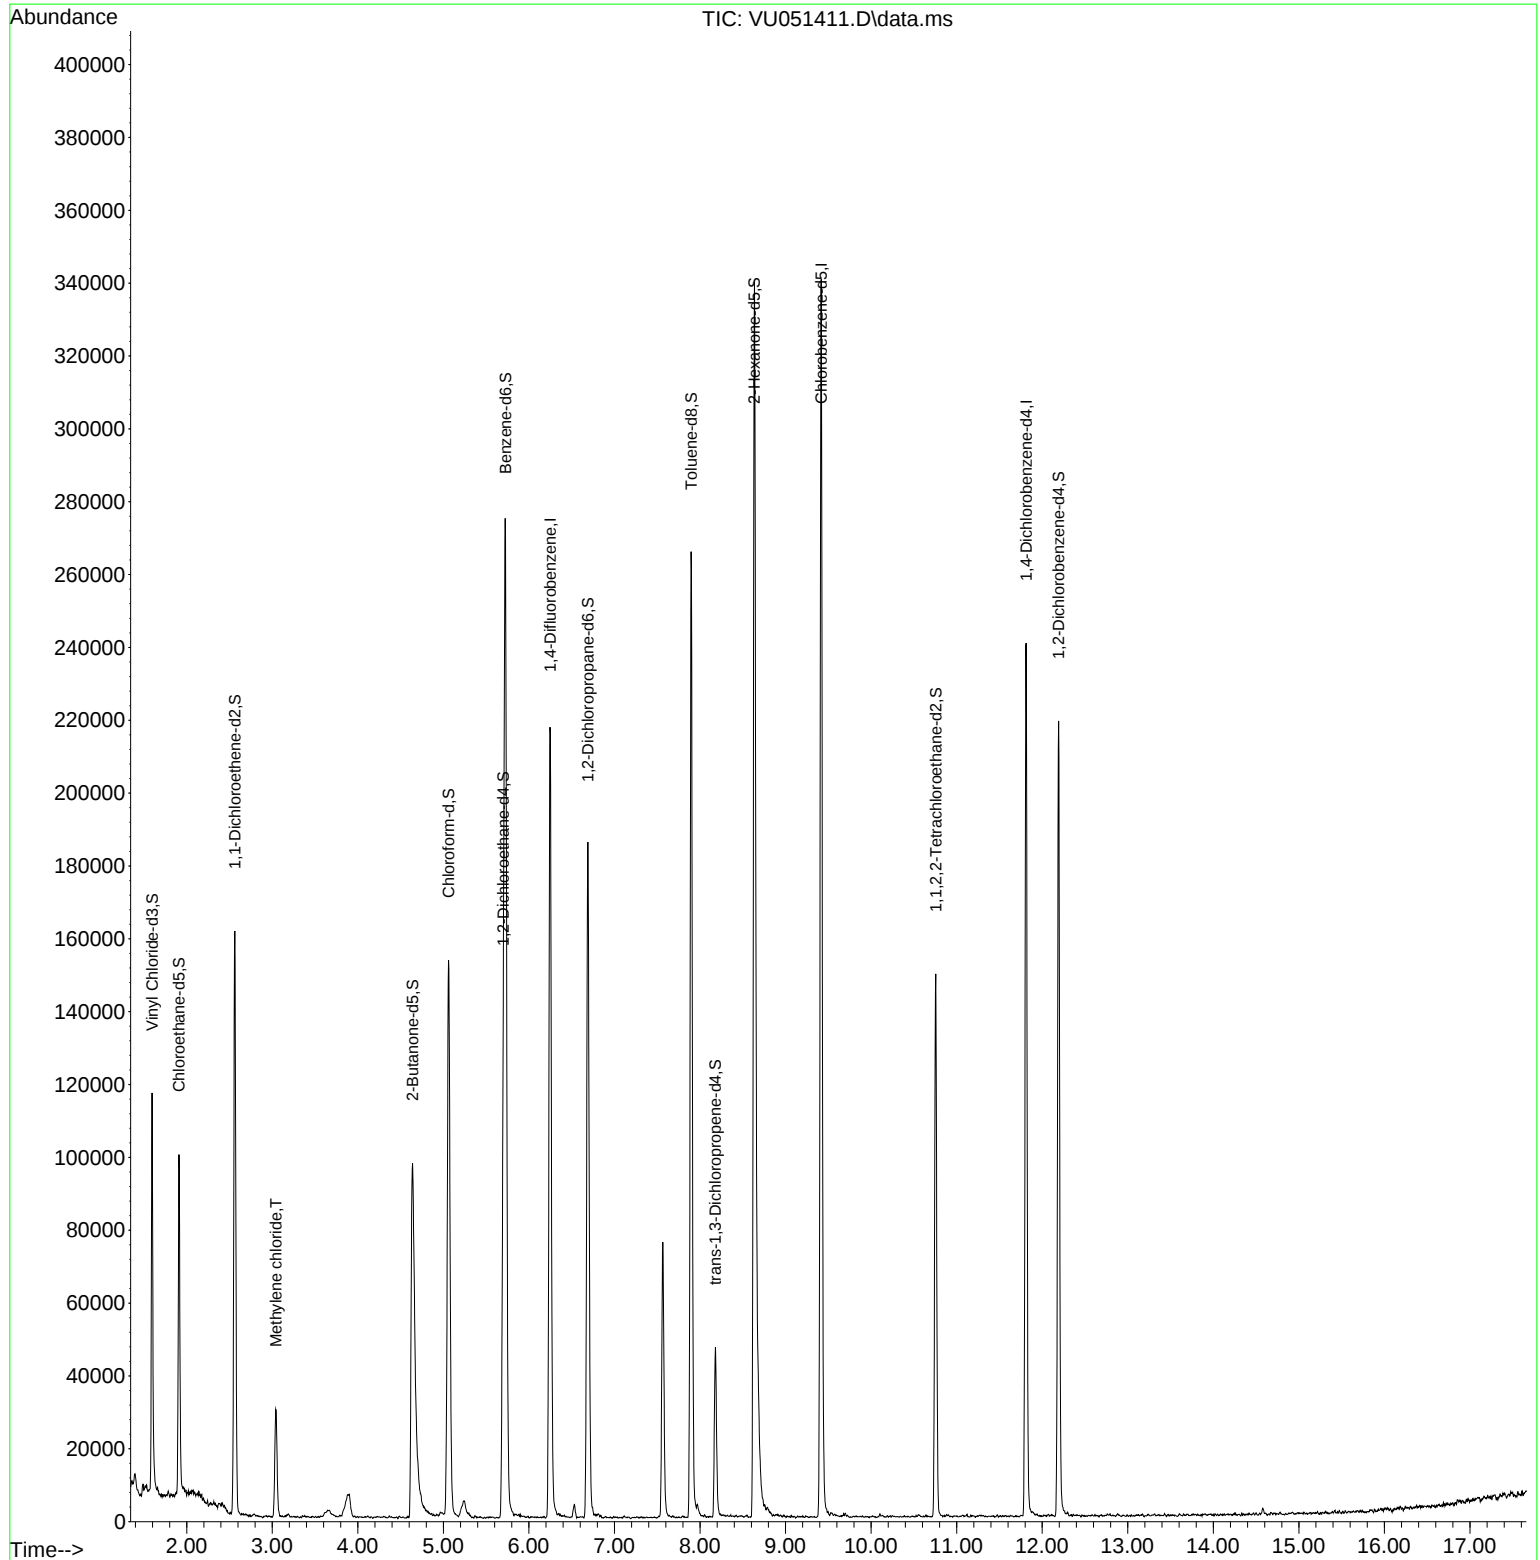

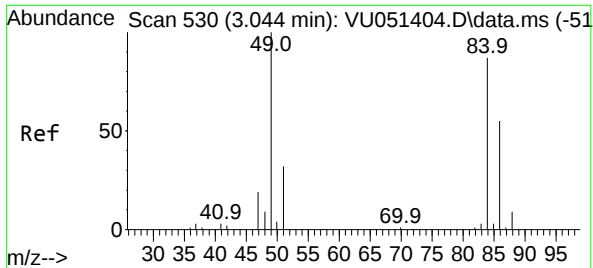

#16
Methylene chloride
Concen: 0.793 ug/L
RT: 3.041 min Scan# 51
Delta R.T. -0.003 min
Lab File: VU051411.D
Acq: 13 Oct 2022 16:43

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

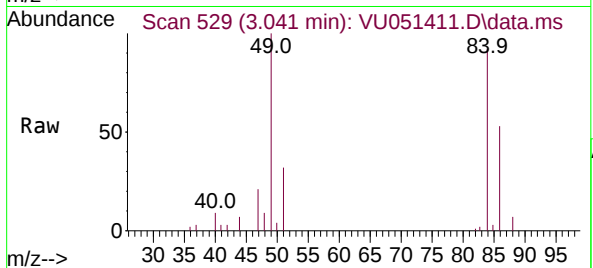

Tgt Ion:	84	Resp:	14815
Ion	Ratio	Lower	Upper
84	100		
86	58.0	46.5	86.3
49	109.2	81.3	151.1

