

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101322\
 Data File : VU051412.D
 Acq On : 13 Oct 2022 17:06
 Operator : JC/MD
 Sample : N5024-12
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Oct 14 01:22:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 14 01:20:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	183576	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	203746	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	67463	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	75126	5.073	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	101.400%	
7) Chloroethane-d5	1.909	69	64543	5.073	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	101.400%	
11) 1,1-Dichloroethene-d2	2.562	65	27714	4.735	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	94.600%	
20) 2-Butanone-d5	4.633	46	146510	44.938	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	89.880%	
24) Chloroform-d	5.060	84	135973	4.925	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.600%	
26) 1,2-Dichloroethane-d4	5.700	65	73146	5.138	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	102.800%	
32) Benzene-d6	5.726	84	242472	4.326	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.600%	
36) 1,2-Dichloropropane-d6	6.690	67	87897	4.617	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	92.400%	
41) Toluene-d8	7.896	98	169699	3.384	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	67.600%#	
43) trans-1,3-Dichloroprop...	8.179	79	26038	4.163	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	83.200%	
46) 2-Hexanone-d5	8.636	63	80744	38.308	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	76.620%	
56) 1,1,2,2-Tetrachloroeth...	10.754	84	65862	4.331	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	86.600%	
66) 1,2-Dichlorobenzene-d4	12.192	152	53736	4.583	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	91.600%	
Target Compounds						
					Qvalue	
13) Acetone	2.645	43	8556	3.499	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101322\
Data File : VU051412.D
Acq On : 13 Oct 2022 17:06
Operator : JC/MD
Sample : N5024-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Time: Oct 14 01:22:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 14 01:20:41 2022
Response via : Initial Calibration

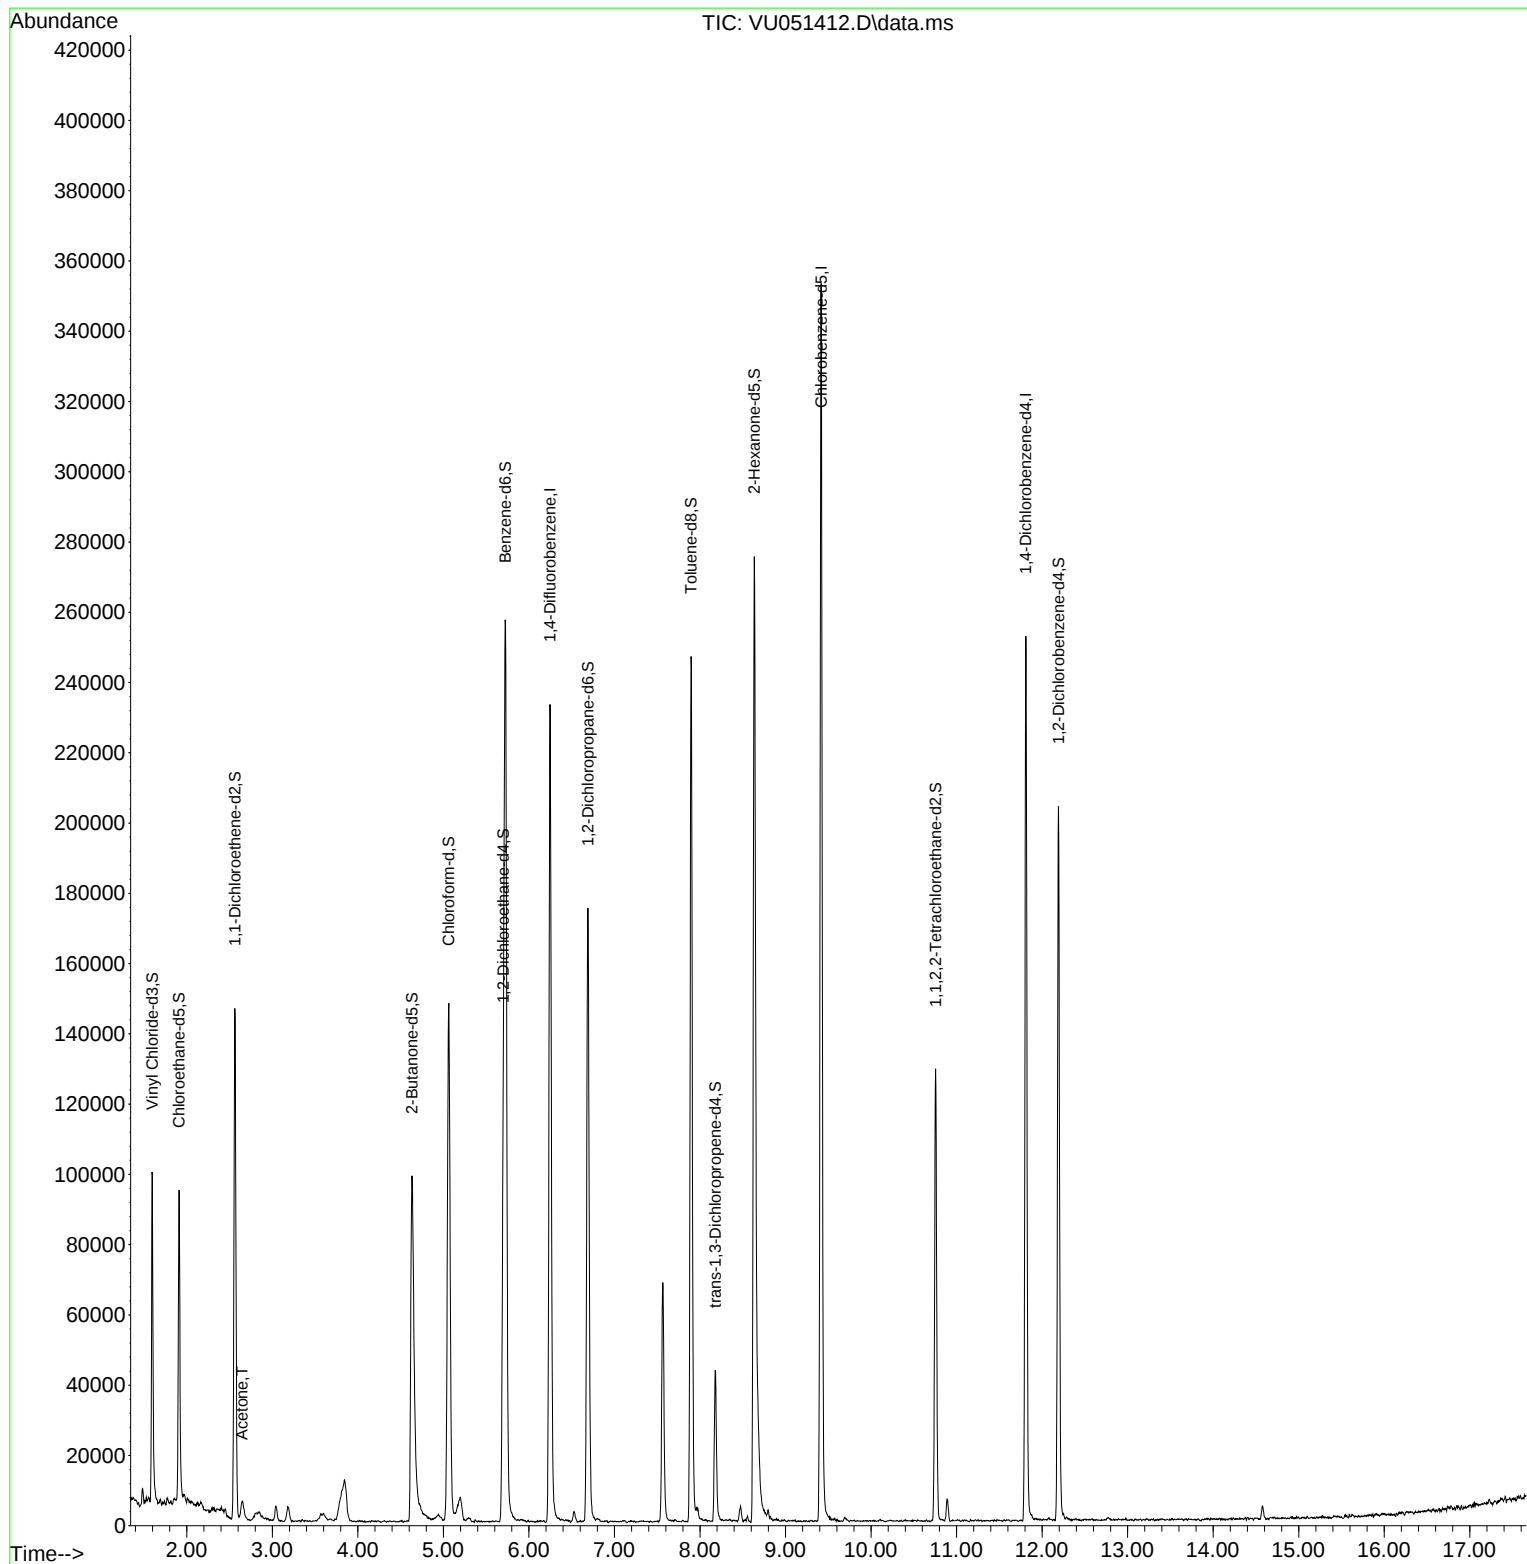

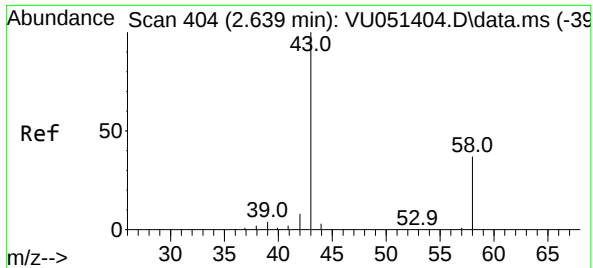

#13
 Acetone
 Concen: 3.499 ug/L
 RT: 2.645 min Scan# 40
 Delta R.T. 0.006 min
 Lab File: VU051412.D
 Acq: 13 Oct 2022 17:06

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Tgt Ion: 43 Resp: 8556
 Ion Ratio Lower Upper
 43 100
 58 32.9 0.0 68.8

