

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101322\
 Data File : VU051414.D
 Acq On : 13 Oct 2022 17:54
 Operator : JC/MD
 Sample : N5023-18
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BE2

Quant Time: Oct 14 01:23:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 14 01:20:41 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		6.247	114	187337	5.000	ug/L	0.00
28) Chlorobenzene-d5		9.414	117	208939	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.809	152	71885	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.594	65	77800	5.148	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	103.000%	
7) Chloroethane-d5		1.909	69	64558	4.972	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.400%	
11) 1,1-Dichloroethene-d2		2.562	65	30058	5.032	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	100.600%	
20) 2-Butanone-d5		4.636	46	174514	52.453	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.900%	
24) Chloroform-d		5.060	84	142249	5.049	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.000%	
26) 1,2-Dichloroethane-d4		5.703	65	78627	5.412	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.200%	
32) Benzene-d6		5.726	84	248630	4.326	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.600%	
36) 1,2-Dichloropropane-d6		6.690	67	91533	4.689	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.800%	
41) Toluene-d8		7.896	98	174694	3.397	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	68.000%#	
43) trans-1,3-Dichloroprop...		8.179	79	27123	4.229	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.600%	
46) 2-Hexanone-d5		8.632	63	100612	46.547	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.100%	
56) 1,1,2,2-Tetrachloroeth...		10.755	84	75525	4.843	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.800%	
66) 1,2-Dichlorobenzene-d4		12.192	152	58855	4.711	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.200%	
Target Compounds							
13) Acetone		2.649	43	8632	3.459	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101322\
Data File : VU051414.D
Acq On : 13 Oct 2022 17:54
Operator : JC/MD
Sample : N5023-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BE2

Quant Time: Oct 14 01:23:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 14 01:20:41 2022
Response via : Initial Calibration

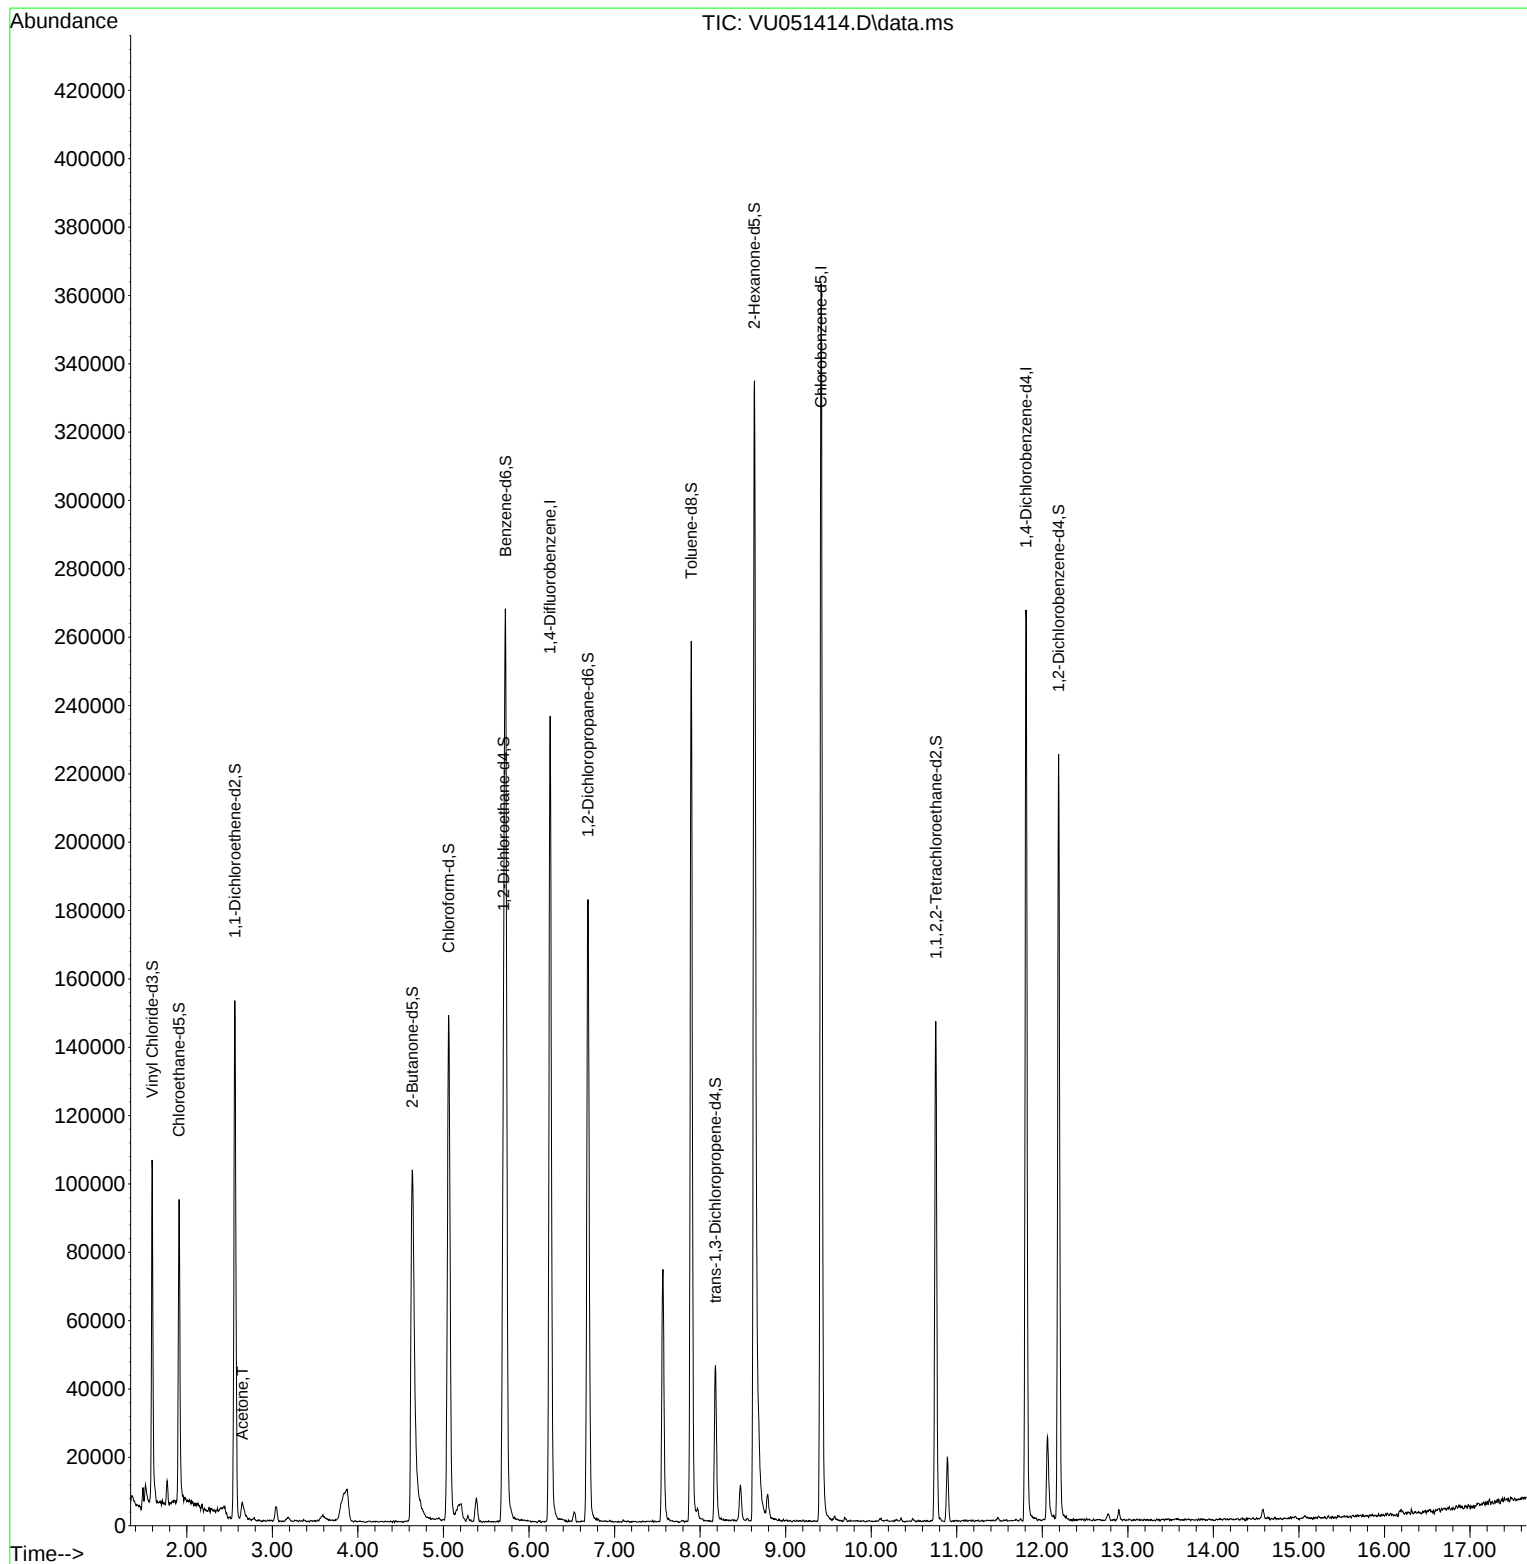

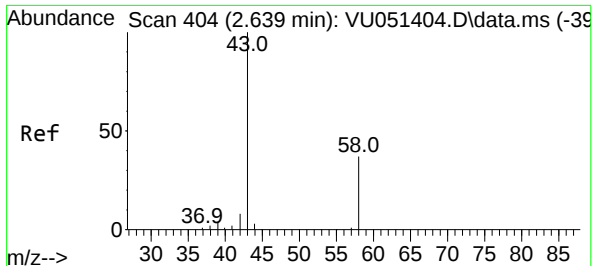

#13

Acetone

Concen: 3.459 ug/L

RT: 2.649 min Scan# 40

Delta R.T. 0.010 min

Lab File: VU051414.D


Acq: 13 Oct 2022 17:54

Instrument :

MSVOA_U

ClientSampleId :

C0BE2

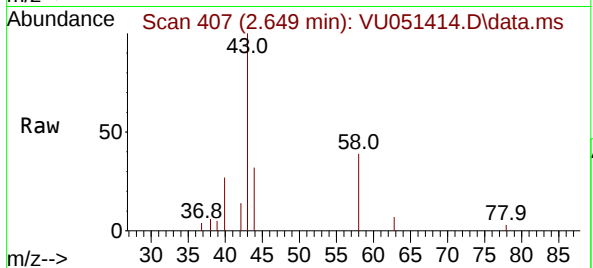

Tgt Ion: 43 Resp: 8632

Ion Ratio Lower Upper

43 100

58 33.1 0.0 68.8

