

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101322\
 Data File : VU051415.D
 Acq On : 13 Oct 2022 18:18
 Operator : JC/MD
 Sample : N5070-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Oct 14 01:23:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 14 01:20:41 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		6.250	114	188858	5.000	ug/L	0.00
28) Chlorobenzene-d5		9.417	117	208882	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.812	152	73240	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.594	65	82081	5.388	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	107.800%	
7) Chloroethane-d5		1.909	69	71721	5.479	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	109.600%	
11) 1,1-Dichloroethene-d2		2.562	65	30562	5.075	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	101.600%	
20) 2-Butanone-d5		4.636	46	186404	55.576	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.160%	
24) Chloroform-d		5.060	84	150034	5.283	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.600%	
26) 1,2-Dichloroethane-d4		5.700	65	82244	5.615	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.400%	
32) Benzene-d6		5.726	84	259591	4.518	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.400%	
36) 1,2-Dichloropropane-d6		6.690	67	97316	4.987	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.800%	
41) Toluene-d8		7.896	98	188397	3.665	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.200%	
43) trans-1,3-Dichloroprop...		8.179	79	29447	4.593	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.800%	
46) 2-Hexanone-d5		8.635	63	110705	51.231	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.460%	
56) 1,1,2,2-Tetrachloroeth...		10.754	84	80818	5.184	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.600%	
66) 1,2-Dichlorobenzene-d4		12.192	152	64496	5.067	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.400%	
Target Compounds							Qvalue
13) Acetone		2.655	43	13672	5.435	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101322\
Data File : VU051415.D
Acq On : 13 Oct 2022 18:18
Operator : JC/MD
Sample : N5070-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Time: Oct 14 01:23:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 14 01:20:41 2022
Response via : Initial Calibration

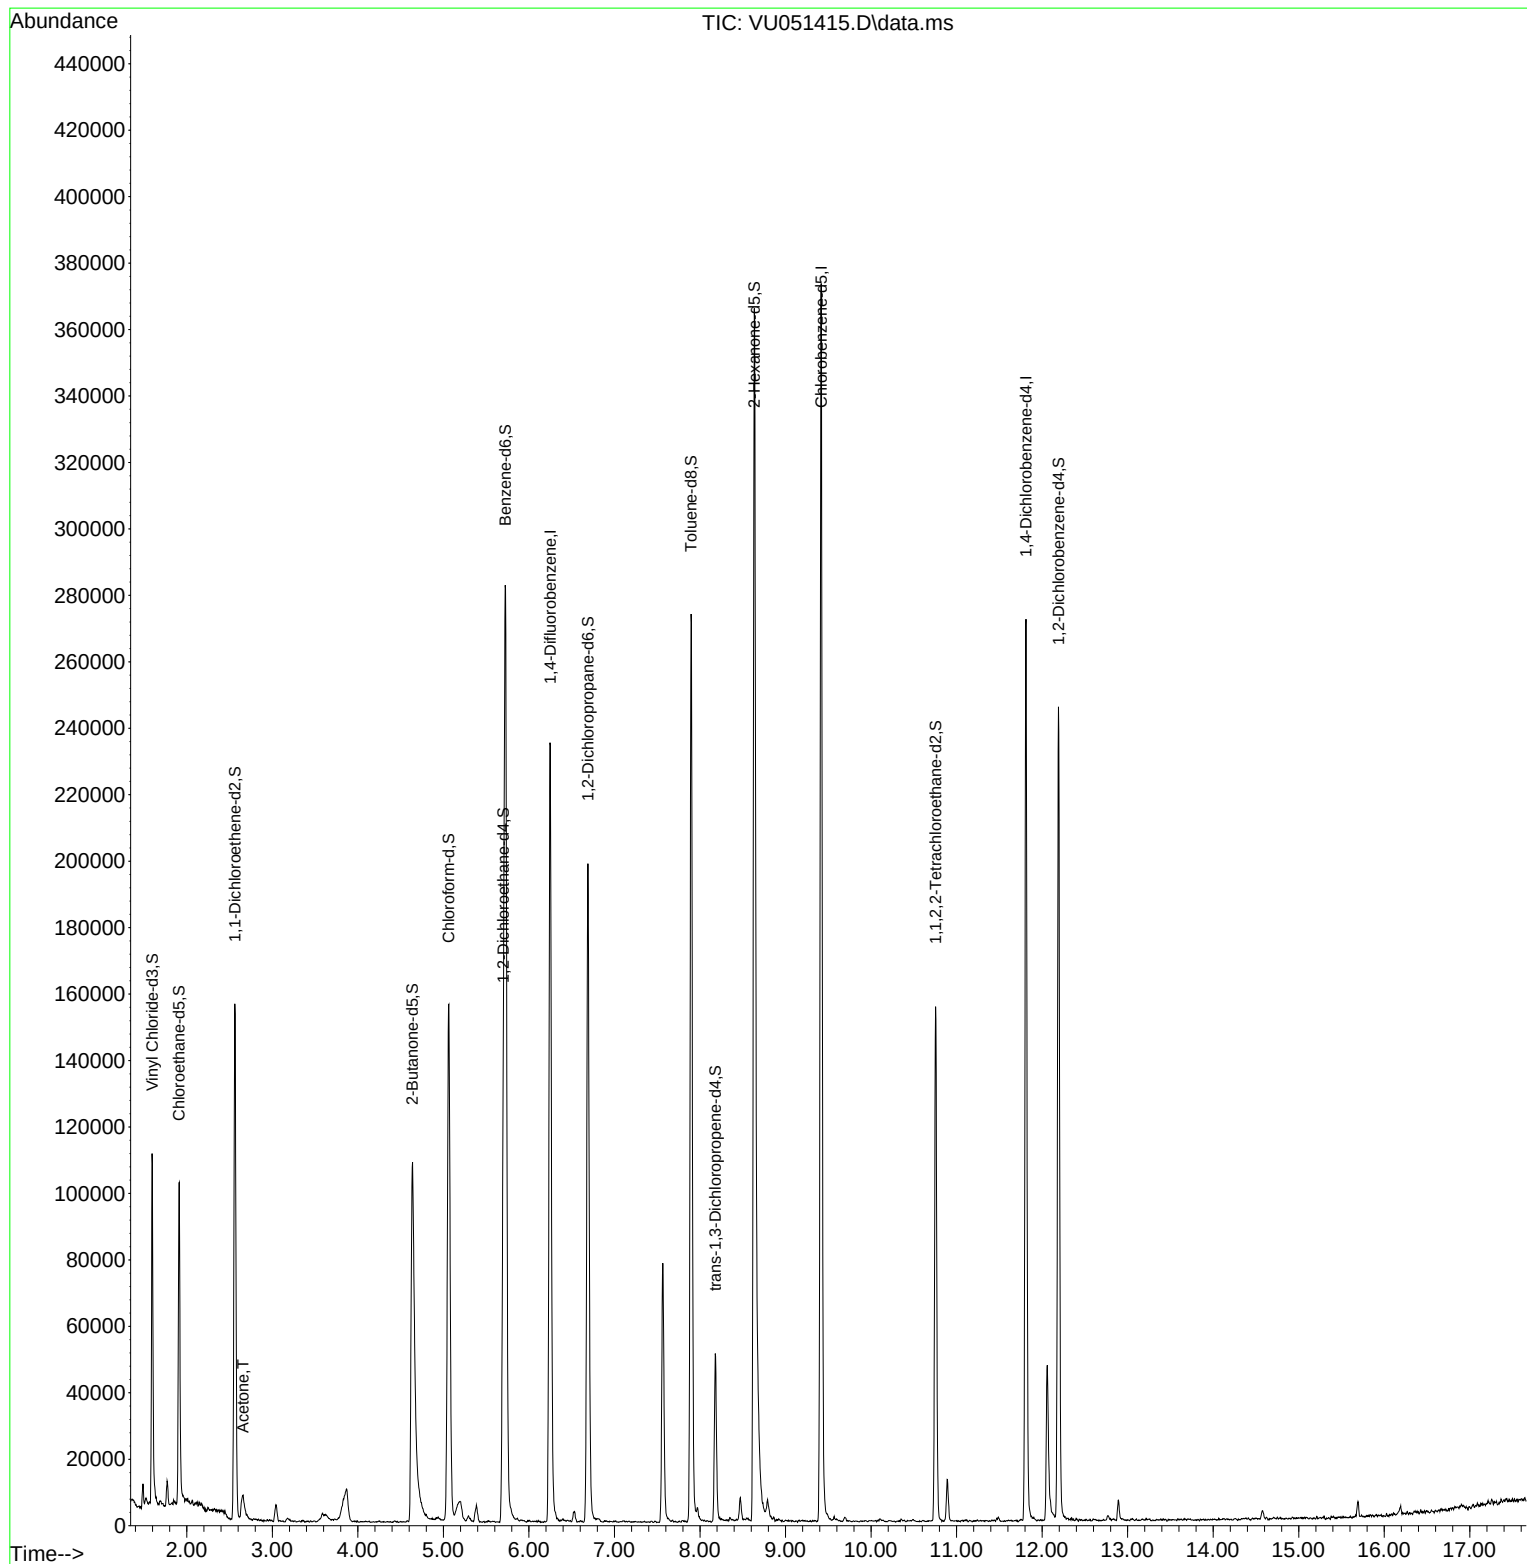

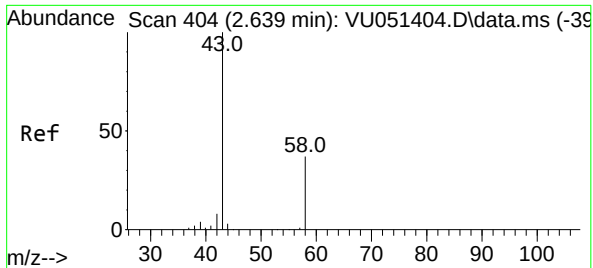

#13
 Acetone
 Concen: 5.435 ug/L
 RT: 2.655 min Scan# 40
 Delta R.T. 0.016 min
 Lab File: VU051415.D
 Acq: 13 Oct 2022 18:18

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Tgt Ion: 43 Resp: 13672
 Ion Ratio Lower Upper
 43 100
 58 32.4 0.0 68.8

