

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101322\
 Data File : VU051416.D
 Acq On : 13 Oct 2022 18:43
 Operator : JC/MD
 Sample : N4993-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Oct 14 01:23:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 14 01:20:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	186965	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	208100	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	72434	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	76645	5.082	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.600%
7) Chloroethane-d5	1.909	69	61918	4.778	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.600%
11) 1,1-Dichloroethene-d2	2.562	65	28998	4.864	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	97.200%
20) 2-Butanone-d5	4.639	46	177227	53.375	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.740%
24) Chloroform-d	5.063	84	138780	4.936	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.800%
26) 1,2-Dichloroethane-d4	5.703	65	74942	5.168	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.400%
32) Benzene-d6	5.726	84	241206	4.213	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.200%
36) 1,2-Dichloropropane-d6	6.690	67	89474	4.602	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.000%
41) Toluene-d8	7.896	98	173116	3.380	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	67.600%#
43) trans-1,3-Dichloroprop...	8.179	79	27145	4.250	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.000%
46) 2-Hexanone-d5	8.636	63	100828	46.835	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.680%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	74193	4.777	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.600%
66) 1,2-Dichlorobenzene-d4	12.192	152	60595	4.813	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.200%
Target Compounds					Qvalue	
13) Acetone	2.652	43	10237	4.111	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101322\
Data File : VU051416.D
Acq On : 13 Oct 2022 18:43
Operator : JC/MD
Sample : N4993-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Time: Oct 14 01:23:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 14 01:20:41 2022
Response via : Initial Calibration

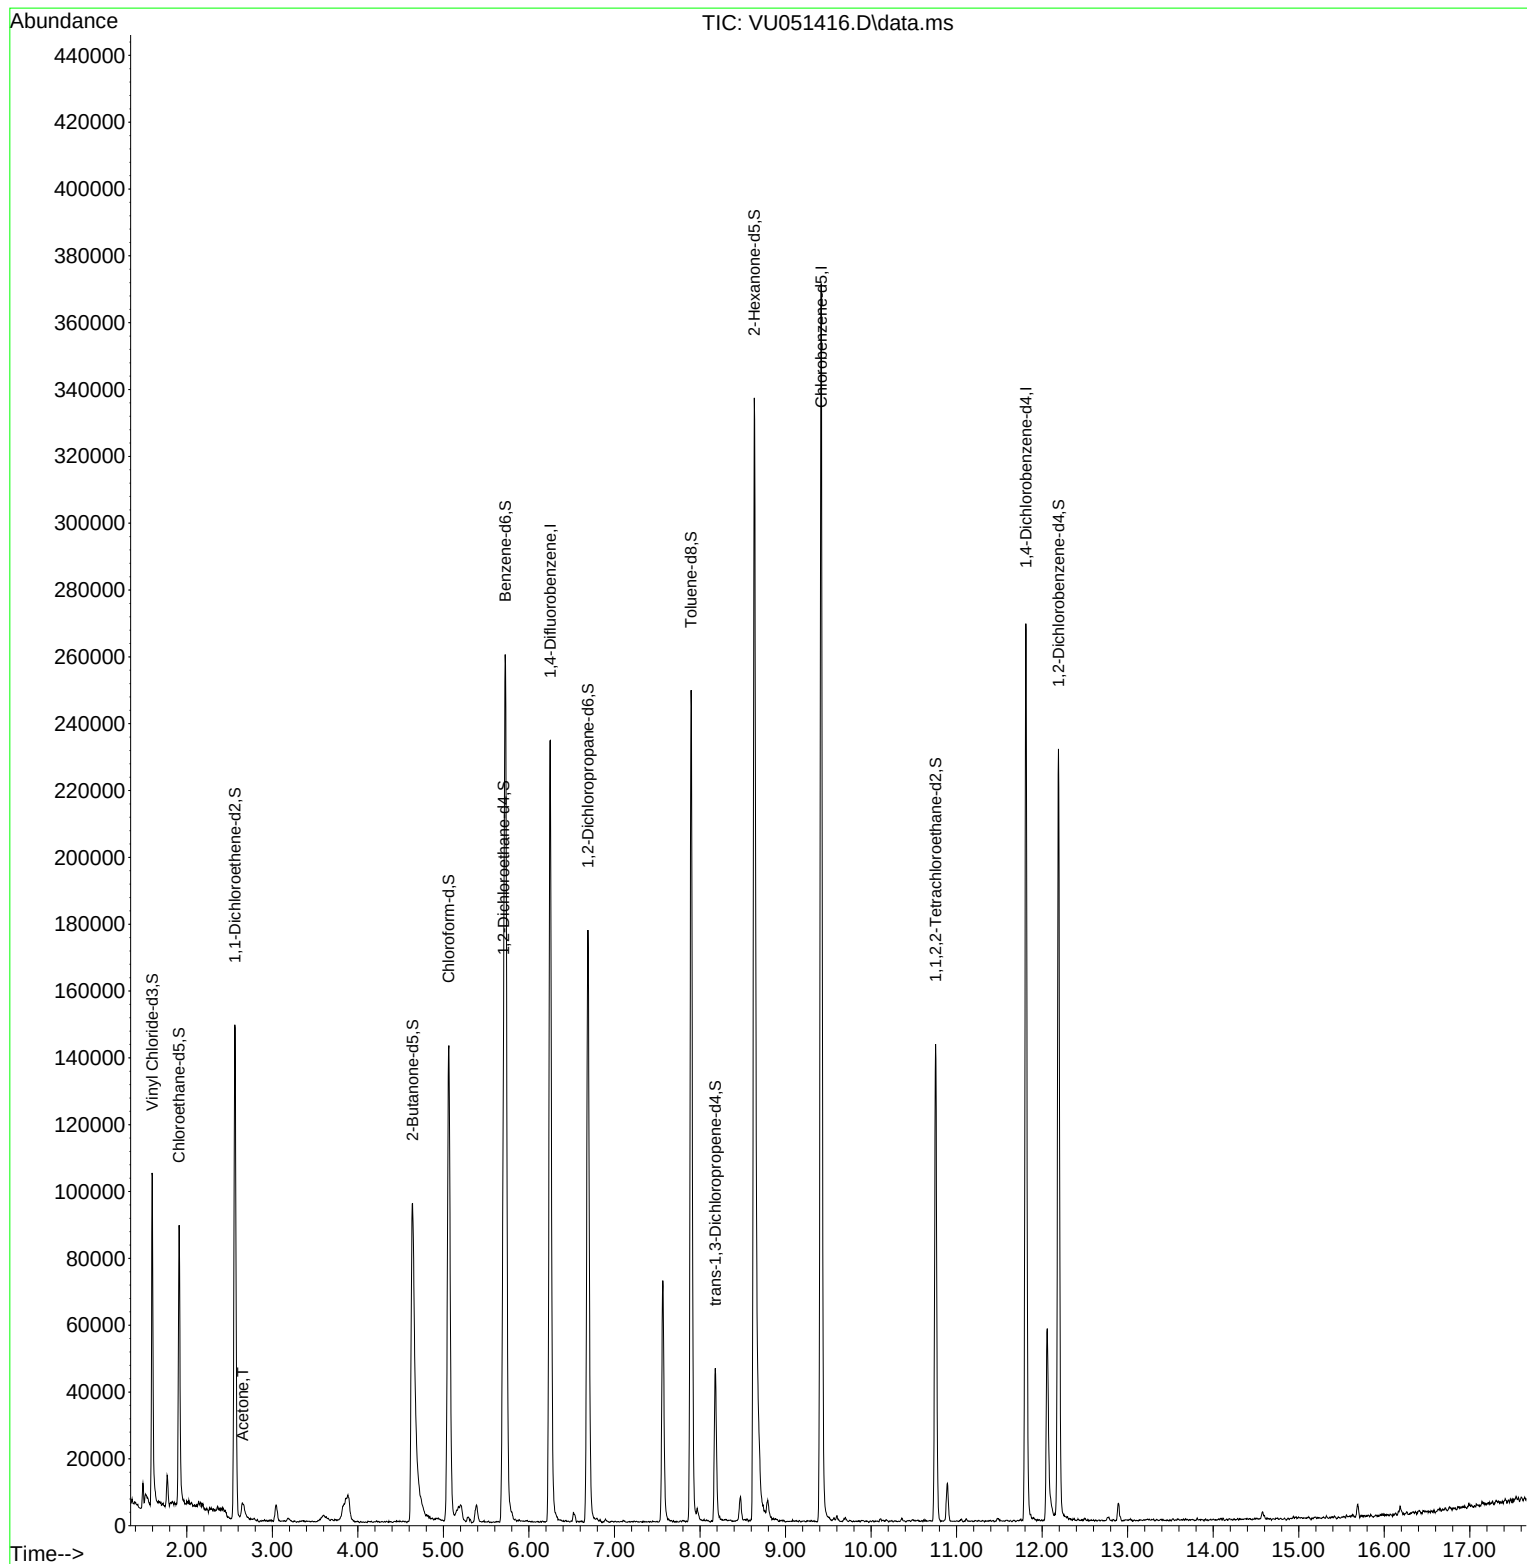

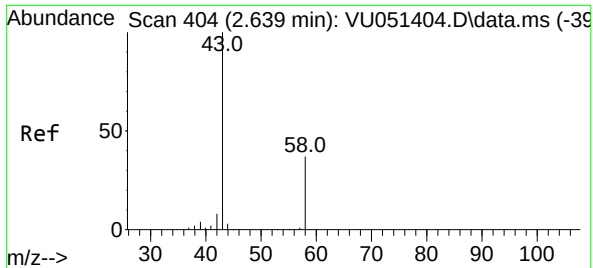

#13
 Acetone
 Concen: 4.111 ug/L
 RT: 2.652 min Scan# 40
 Delta R.T. 0.013 min
 Lab File: VU051416.D
 Acq: 13 Oct 2022 18:43

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Tgt Ion: 43 Resp: 10237
 Ion Ratio Lower Upper
 43 100
 58 32.7 0.0 68.8

