

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101322\
 Data File : VU051413.D
 Acq On : 13 Oct 2022 17:31
 Operator : JC/MD
 Sample : N5026-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051413.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	72	79	95	rBV	95829	112808	15.63%	1.979%
2	1.909	168	177	195	rBV	88733	120005	16.63%	2.105%
3	2.562	369	380	396	rBV	146680	240180	33.28%	4.213%
4	2.645	396	406	427	rVB3	5029	13161	1.82%	0.231%
5	3.182	561	573	585	rBV3	3581	8355	1.16%	0.147%
6	3.819	751	771	772	rBV2	7632	17475	2.42%	0.307%
7	4.636	1012	1025	1061	rBV	106806	325537	45.10%	5.710%
8	5.060	1141	1157	1190	rBV	152623	357657	49.56%	6.273%
9	5.723	1343	1363	1395	rBV2	261662	697006	96.57%	12.225%
10	6.247	1512	1526	1548	rBV	231424	448322	62.12%	7.864%
11	6.690	1650	1664	1682	rBV	180766	350694	48.59%	6.151%
12	7.565	1923	1936	1955	rBV2	73882	131416	18.21%	2.305%
13	7.896	2027	2039	2057	rBV	246304	437306	60.59%	7.670%
14	8.179	2112	2127	2143	rBV	46248	79439	11.01%	1.393%
15	8.472	2204	2218	2230	rBV3	8191	15290	2.12%	0.268%
16	8.636	2255	2269	2305	rBV2	326972	721737	100.00%	12.659%
17	9.417	2499	2512	2537	rBV	357493	605432	83.89%	10.619%
18	10.754	2916	2928	2946	rBV	143820	229972	31.86%	4.034%
19	10.893	2959	2971	2980	rBV2	15063	23896	3.31%	0.419%
20	11.812	3244	3257	3277	rBV	254190	418148	57.94%	7.334%
21	12.192	3359	3375	3391	rBV	213056	347454	48.14%	6.094%




Sum of corrected areas: 5701290

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101322\
Data File : VU051413.D
Acq On : 13 Oct 2022 17:31
Operator : JC/MD
Sample : N5026-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

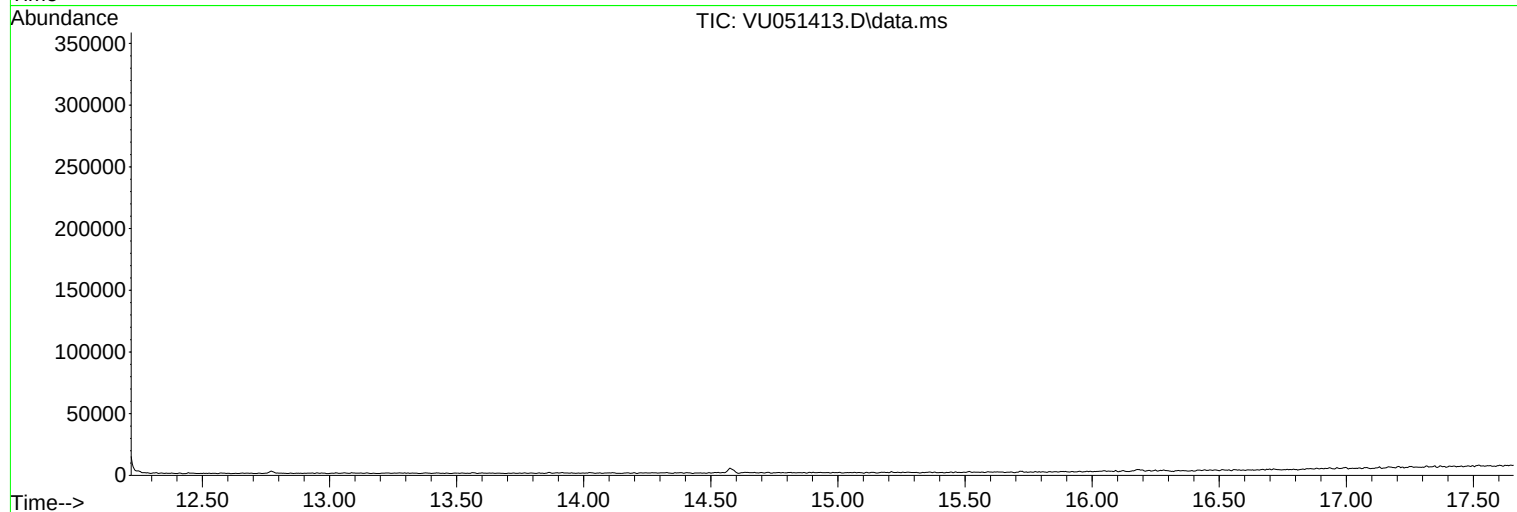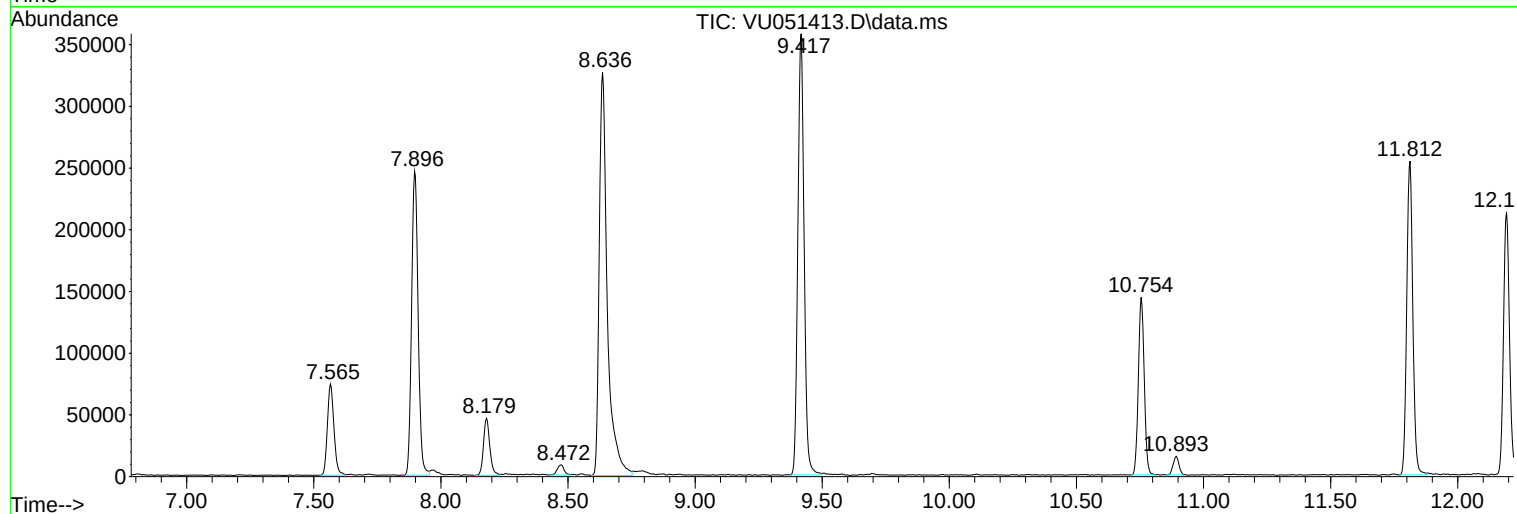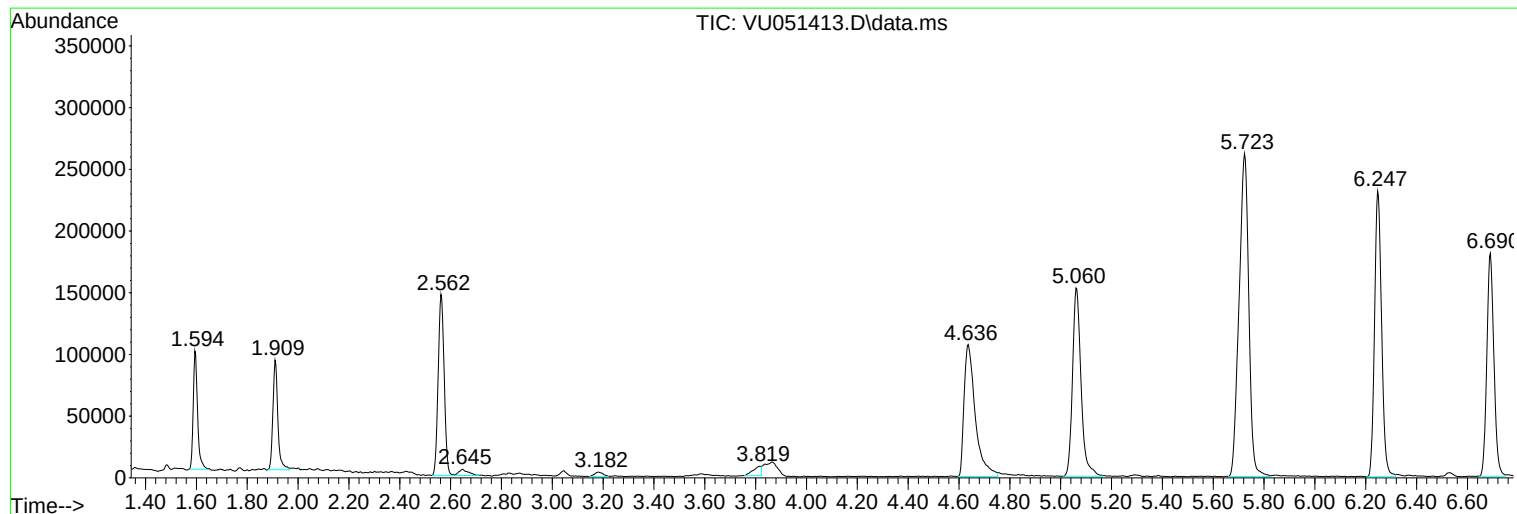

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101322\
Data File : VU051413.D
Acq On : 13 Oct 2022 17:31
Operator : JC/MD
Sample : N5026-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101322\
Data File : VU051413.D
Acq On : 13 Oct 2022 17:31
Operator : JC/MD
Sample : N5026-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc