

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101322\
 Data File : VU051417.D
 Acq On : 13 Oct 2022 19:08
 Operator : JC/MD
 Sample : N5024-12
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051417.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	72	79	100	rVB	112905	136468	17.60%	2.267%
2	1.909	168	177	192	rBV	98679	128404	16.56%	2.133%
3	2.562	369	380	395	rBV	152538	248366	32.03%	4.125%
4	3.044	517	530	544	rBV	37635	69268	8.93%	1.150%
5	3.832	755	775	778	rBV	3608	8098	1.04%	0.135%
6	4.642	1004	1027	1071	rBV	99203	340177	43.86%	5.650%
7	5.063	1141	1158	1175	rBV	151013	333604	43.02%	5.541%
8	5.723	1343	1363	1389	rBV2	275709	737657	95.12%	12.252%
9	6.247	1513	1526	1556	rBV	235999	464479	59.89%	7.715%
10	6.690	1650	1664	1684	rBV	188767	372542	48.04%	6.188%
11	7.565	1924	1936	1958	rBV	76813	138078	17.80%	2.293%
12	7.896	2026	2039	2056	rBV	265656	469756	60.57%	7.802%
13	8.179	2117	2127	2142	rBV2	47219	81653	10.53%	1.356%
14	8.468	2207	2217	2227	rBV3	5326	9084	1.17%	0.151%
15	8.636	2257	2269	2310	rBV2	353267	775533	100.00%	12.881%
16	9.417	2499	2512	2535	rBV	371686	630994	81.36%	10.480%
17	10.755	2916	2928	2947	rBV	152494	247633	31.93%	4.113%
18	10.890	2958	2970	2981	rBV3	7143	12488	1.61%	0.207%
19	11.812	3242	3257	3276	rBV	267567	431449	55.63%	7.166%
20	12.066	3328	3336	3355	rVB6	5453	11208	1.45%	0.186%
21	12.192	3363	3375	3397	rBV	227834	373749	48.19%	6.208%




Sum of corrected areas: 6020688

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101322\
Data File : VU051417.D
Acq On : 13 Oct 2022 19:08
Operator : JC/MD
Sample : N5024-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

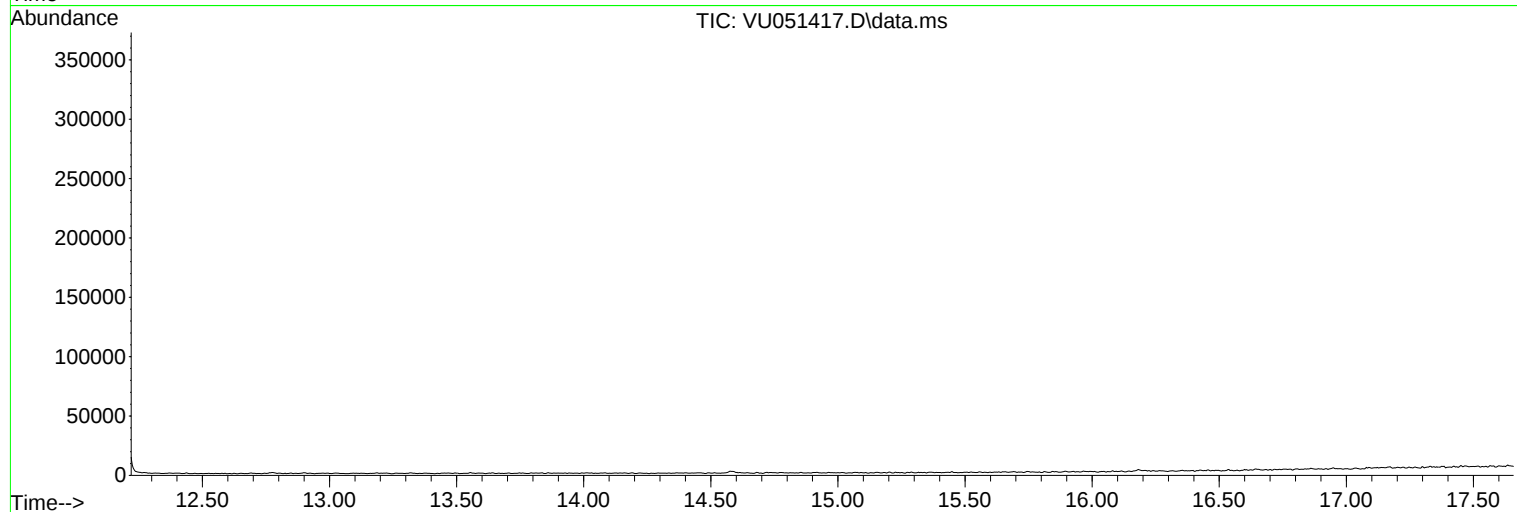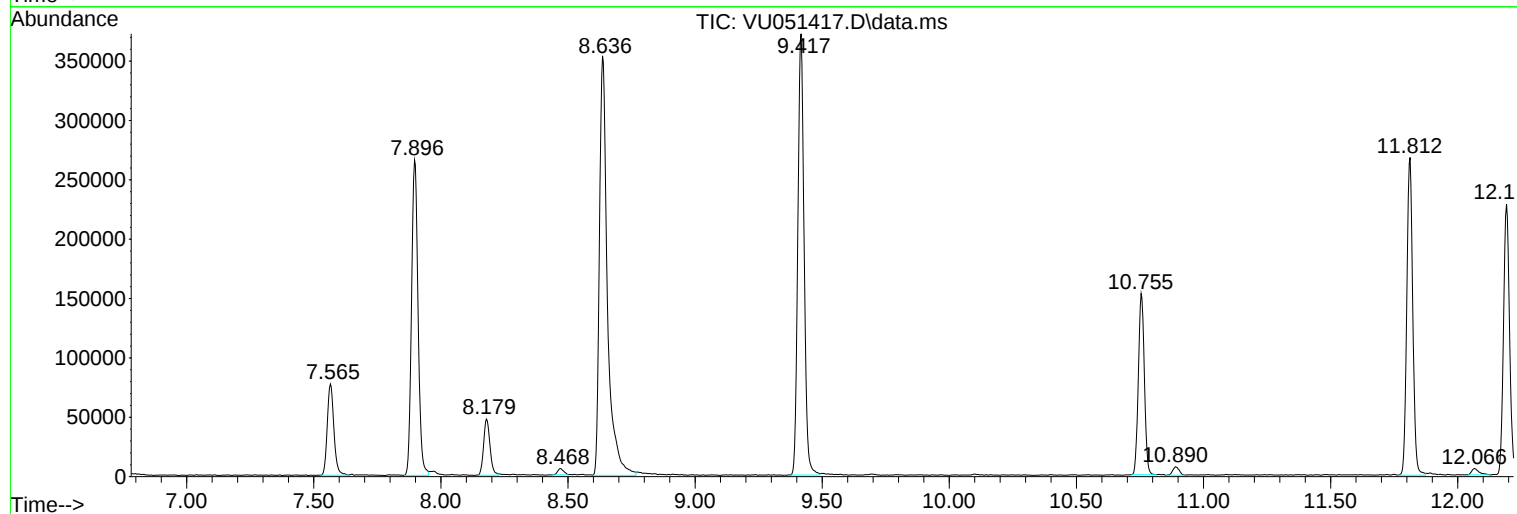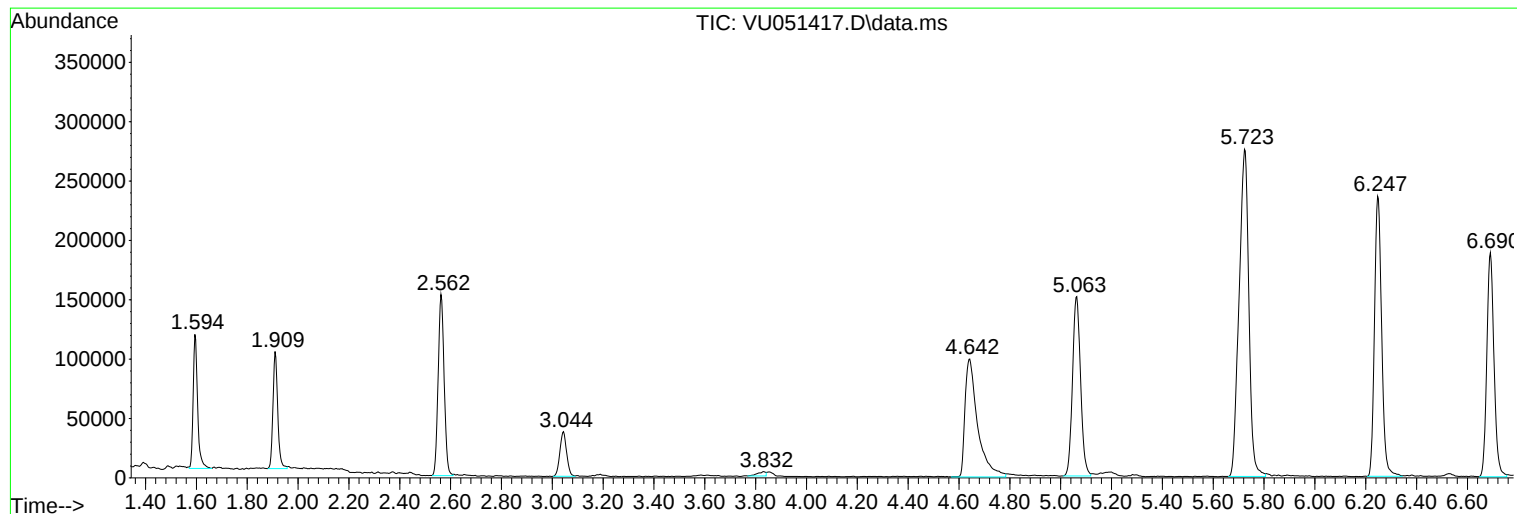

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101322\
Data File : VU051417.D
Acq On : 13 Oct 2022 19:08
Operator : JC/MD
Sample : N5024-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101322\
Data File : VU051417.D
Acq On : 13 Oct 2022 19:08
Operator : JC/MD
Sample : N5024-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc