


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101322\
Data File : VU051403.D
Acq On : 13 Oct 2022 09:44
Operator : JC/MD
Sample : BFB156
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB156

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100722WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Oct 14 01:20:41 2022

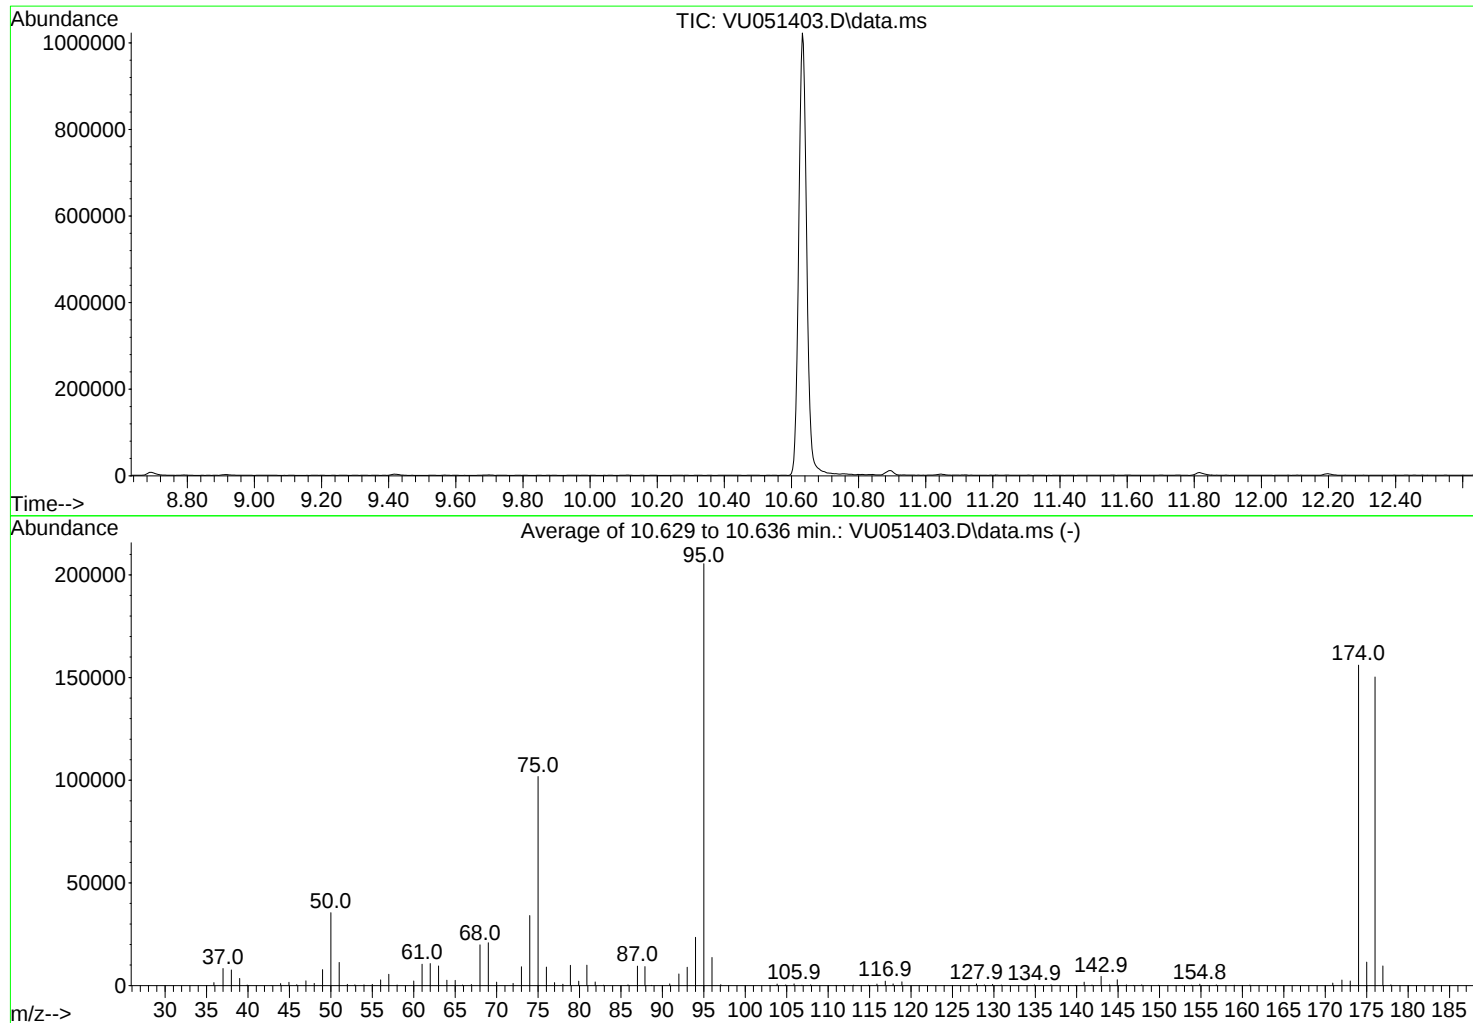

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	35501	PASS
75	95	30	80	49.6	101797	PASS
95	95	100	100	100.0	205419	PASS
96	95	5	9	6.7	13687	PASS
173	174	0.00	2	1.4	2244	PASS
174	95	50	120	76.0	156032	PASS
175	174	5	9	7.3	11434	PASS
176	174	95	101	96.3	150251	PASS
177	176	5	9	6.4	9556	PASS

m/z	Abundance
39.90	731.0
44.00	531.0

Instrument :
MSVOA_U
ClientSampleId :
BFB156

m/z	Abundance
35.90	1438.0
37.00	8110.0
38.00	7771.0
39.00	3312.0
39.90	958.0
44.00	1482.0
45.00	1473.0
45.90	385.0
47.00	2244.0
48.00	1076.0
49.00	7429.0
50.00	34688.0
51.00	11230.0
52.00	486.0
52.90	367.0
54.00	373.0
55.00	736.0
56.00	2620.0
57.00	5241.0
58.00	336.0
60.00	2174.0
61.00	9936.0
62.00	10361.0
63.00	9558.0
64.00	2587.0
65.00	2379.0
65.90	259.0
66.90	486.0
68.00	19480.0
69.00	20176.0
70.00	1742.0
72.00	1048.0
73.00	8883.0
74.00	33216.0
75.00	98880.0
76.00	9087.0
77.00	1334.0
78.00	628.0
78.90	10013.0
79.90	2027.0
80.90	10012.0
81.90	1627.0
82.90	242.0
85.90	332.0
87.00	8920.0
87.90	8964.0
90.90	719.0
92.00	5612.0
93.00	8524.0
94.00	22592.0
95.00	197760.0
96.00	13351.0
97.10	370.0
103.00	104.0
103.90	742.0
104.90	341.0
105.90	781.0
107.00	211.0
107.90	336.0
111.00	191.0
111.80	188.0
113.10	170.0
114.90	252.0
115.90	653.0
116.90	2050.0
117.90	842.0
118.90	1908.0
127.90	714.0
128.90	319.0
129.80	593.0
130.90	264.0
134.90	273.0
136.90	381.0
139.90	122.0
140.90	1689.0
141.80	219.0
143.00	4623.0
143.90	377.0
144.90	2775.0
146.00	328.0
146.90	151.0
147.90	390.0
149.90	249.0
153.80	193.0
154.80	612.0
156.80	383.0
159.00	202.0
160.90	205.0
170.90	1213.0
172.00	2503.0
173.00	2054.0
174.00	147328.0

Instrument :
MSVOA_U
ClientSampleId :
BFB156

175.00	11004.0
176.00	141760.0
176.90	9546.0
177.90	298.0

Instrument :
MSVOA_U
ClientSampleId :
BFB156

m/z	Abundance
35.90	1457.0
37.00	8603.0
38.00	7838.0
39.00	3612.0
39.90	1058.0
42.80	100.0
43.90	1535.0
45.00	1670.0
45.90	447.0
47.00	2280.0
48.00	1090.0
49.00	7960.0
50.00	36680.0
51.00	11654.0
52.00	576.0
52.90	347.0
54.00	379.0
55.00	667.0
56.00	2838.0
57.00	5678.0
58.00	319.0
60.00	2260.0
61.00	10705.0
62.00	11004.0
63.00	9733.0
64.00	2694.0
65.00	2624.0
65.90	288.0
67.00	489.0
68.00	20400.0
69.00	21480.0
70.00	1800.0
72.00	1057.0
73.00	9396.0
74.00	35496.0
75.00	105016.0
76.00	9180.0
77.00	1470.0
78.00	645.0
78.90	9940.0
79.90	2221.0
80.90	10243.0
81.90	1740.0
82.90	230.0
85.90	373.0
87.00	9784.0
87.90	9653.0
88.70	202.0
90.90	862.0
92.00	5831.0
93.00	9178.0
94.00	24368.0
95.00	211584.0
96.00	14182.0
97.00	401.0
103.80	780.0
104.90	408.0
105.90	838.0
106.80	182.0
107.90	351.0
110.90	142.0
111.80	164.0
113.10	190.0
114.90	239.0
115.90	775.0
116.90	2240.0
117.80	872.0
118.90	1956.0
127.90	920.0
128.90	350.0
129.80	629.0
130.90	283.0
134.90	364.0
136.90	395.0
139.90	134.0
140.90	1712.0
141.90	234.0
142.90	4531.0
144.00	356.0
144.90	2999.0
146.00	352.0
146.80	147.0
147.80	412.0
149.90	217.0
152.80	127.0
153.90	183.0
154.90	664.0
156.90	372.0
159.00	231.0
160.90	266.0
170.90	1212.0
172.00	2793.0

Instrument :
MSVOA_U
ClientSampleId :
BFB156

173.00	2267.0
174.00	160704.0
175.00	11799.0
176.00	155520.0
176.90	9819.0
177.90	360.0

Instrument :
MSVOA_U
ClientSampleId :
BFB156

m/z	Abundance
35.90	1398.0
37.00	8311.0
38.00	7143.0
39.00	3484.0
39.90	1086.0
42.80	104.0
43.90	1514.0
44.90	1717.0
45.90	474.0
47.00	2287.0
48.00	1016.0
49.00	7926.0
50.00	35136.0
51.00	10949.0
52.00	607.0
52.90	285.0
54.00	302.0
55.00	489.0
56.00	2851.0
57.00	5477.0
58.00	242.0
60.00	2241.0
61.00	10494.0
62.00	10860.0
63.00	9284.0
64.00	2504.0
65.00	2514.0
65.90	264.0
67.00	492.0
68.00	19704.0
69.00	20872.0
70.00	1577.0
72.00	976.0
73.00	9123.0
74.00	33616.0
75.00	101496.0
76.00	8689.0
77.00	1432.0
78.00	672.0
78.90	9572.0
79.90	2288.0
80.90	9612.0
81.90	1810.0
82.90	210.0
85.80	352.0
87.00	9653.0
87.90	9214.0
88.70	174.0
90.90	951.0
92.00	5441.0
93.00	9108.0
94.00	23584.0
95.00	206912.0
96.00	13529.0
97.00	476.0
103.80	746.0
104.90	410.0
105.90	821.0
106.80	187.0
107.90	324.0
110.90	118.0
111.90	118.0
113.00	174.0
114.90	208.0
115.90	849.0
116.90	2277.0
117.80	843.0
118.90	1710.0
124.00	120.0
127.90	927.0
128.80	339.0
129.90	638.0
130.90	264.0
134.90	400.0
136.90	363.0
139.80	136.0
140.90	1569.0
141.90	276.0
143.00	4208.0
144.00	302.0
144.90	2840.0
146.00	317.0
146.80	137.0
147.80	370.0
149.80	177.0
152.80	159.0
153.80	141.0
154.90	626.0
155.80	102.0
156.90	305.0
159.00	211.0
160.90	270.0

Instrument :
MSVOA_U
ClientSampleId :
BFB156

170.90	1136.0
172.00	2784.0
173.00	2410.0
174.00	160064.0
175.00	11498.0
176.00	153472.0
177.00	9303.0
177.90	318.0

Instrument :
MSVOA_U
ClientSampleId :
BFB156