

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\U101419\
 Data File : VU035167.D
 Acq On : 14 Oct 2019 22:14
 Operator : JC/SP
 Sample : K5317-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CE4

Quant Time: Oct 15 08:47:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 15 07:54:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	139209	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	148211	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.47	152	52607	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	40754	4.95	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.00%
7) Chloroethane-d5	1.68	69	40651	5.29	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.80%
11) 1,1-Dichloroethene-d2	2.26	63	61696	3.56	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.20%
20) 2-Butanone-d5	4.17	46	130519	53.86	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.72%
24) Chloroform-d	4.62	84	75805	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
26) 1,2-Dichloroethane-d4	5.29	65	50303	5.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.20%
32) Benzene-d6	5.32	84	160805	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.60%
36) 1,2-Dichloropropane-d6	6.31	67	58535	5.04	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.80%
41) Toluene-d8	7.55	98	134041	3.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.80%
43) trans-1,3-Dichloropropene-	7.84	79	16457	3.94	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.80%
46) 2-Hexanone-d5	8.31	63	94186	47.36	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.72%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	50913	5.20	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.00%
64) 1,2-Dichlorobenzene-d4	11.85	152	46461	5.24	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.80%


Target Compounds					Qvalue
13) Acetone	2.31	43	4288	2.160 ug/L	91
25) Chloroform	4.65	83	12264	0.574 ug/L	94
47) Tetrachloroethene	8.21	164	4839	0.519 ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101419\
Data File : VU035167.D
Acq On : 14 Oct 2019 22:14
Operator : JC/SP
Sample : K5317-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CE4

Quant Time: Oct 15 08:47:56 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 15 07:54:07 2019
Response via : Initial Calibration

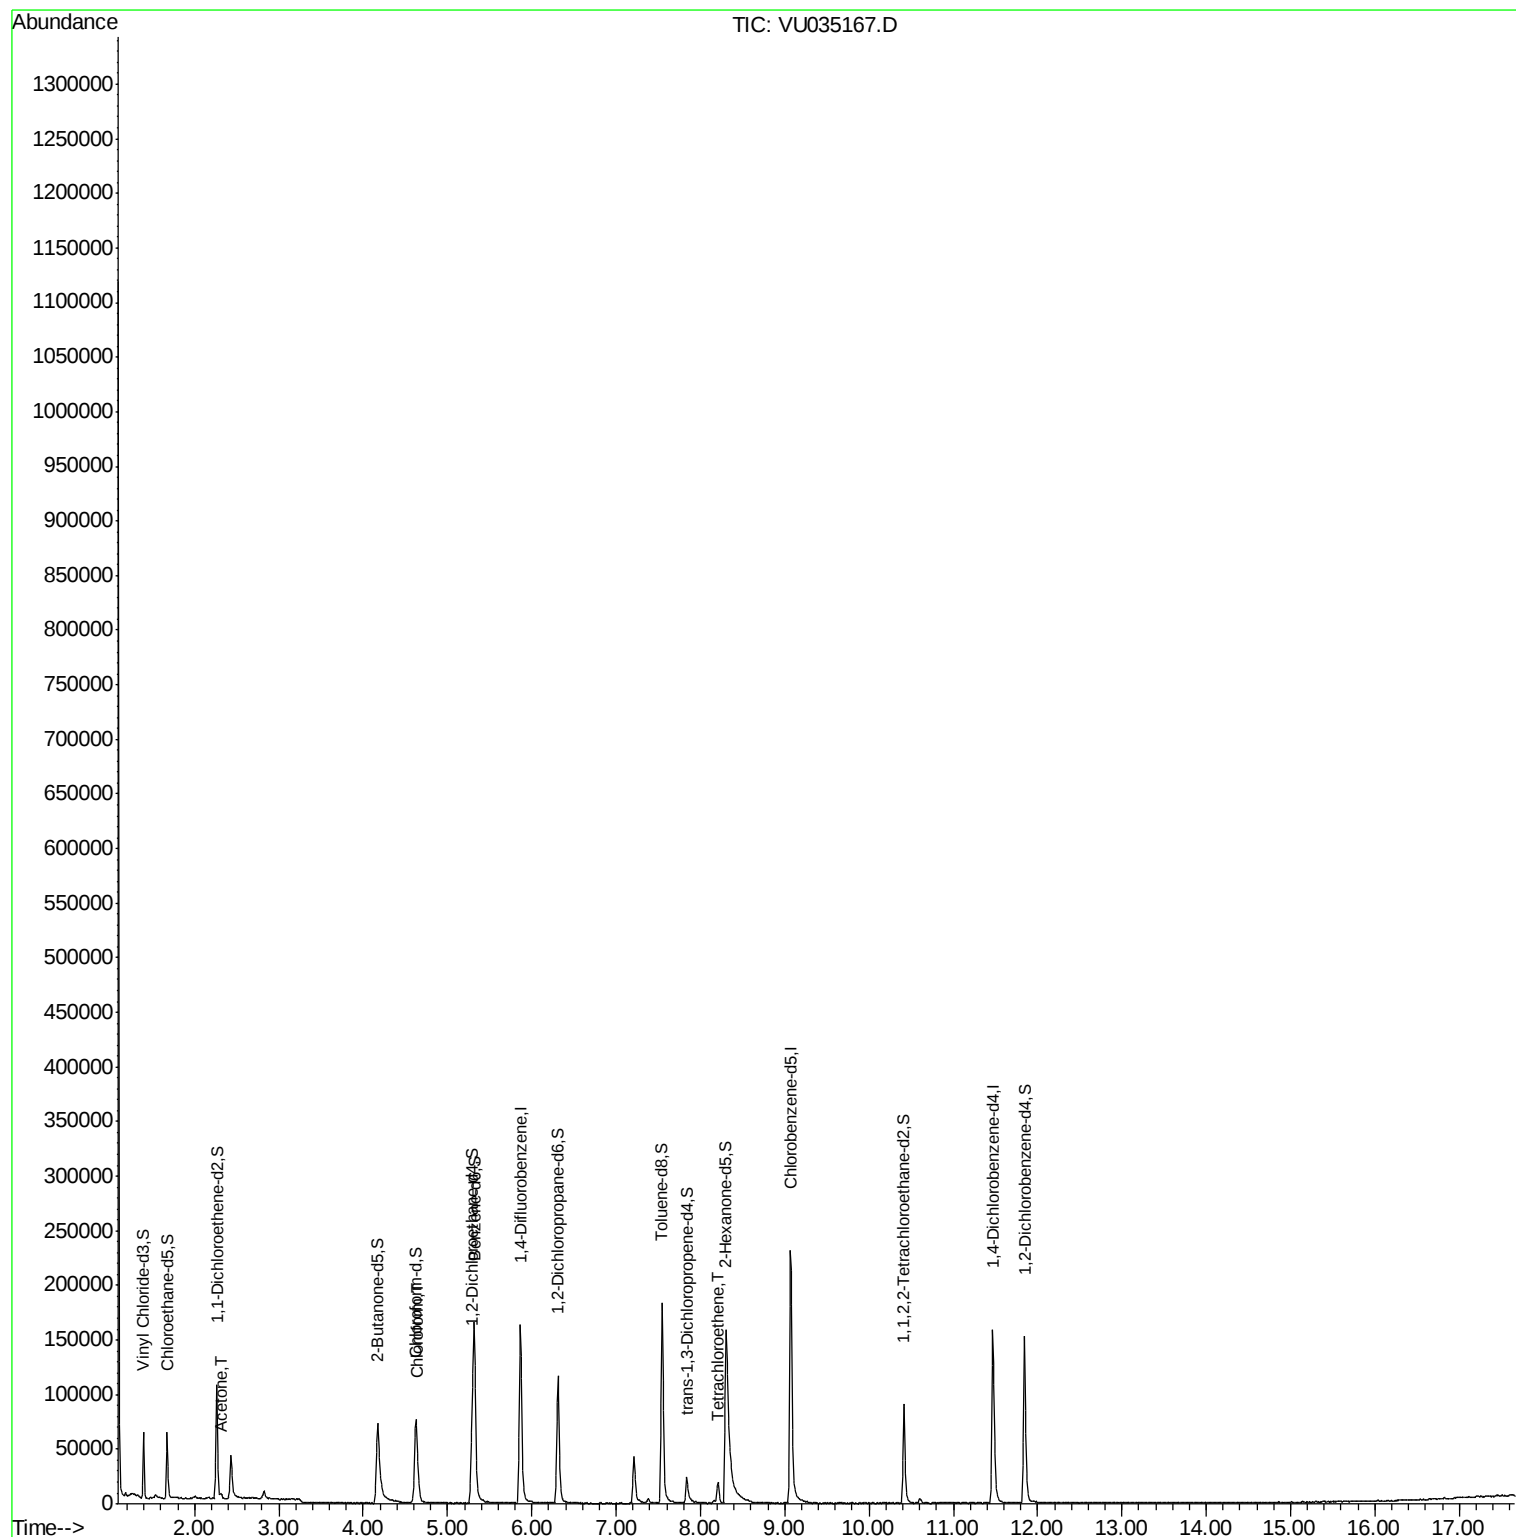

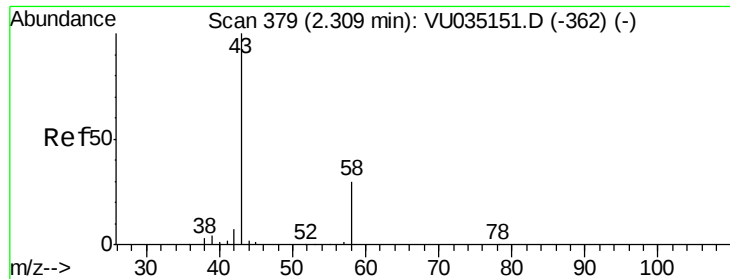

#13

Acetone

Concen: 2.160 ug/L

RT: 2.31 min Scan# 381

Delta R.T. 0.01 min

Lab File: VU035167.D

Acq: 14 Oct 2019 22:14

Instrument :

MSVOA_U

ClientSampleId :


C0CE4

Tgt Ion: 43 Resp: 4288

Ion Ratio Lower Upper

43 100

58 28.1 0.0 66.6

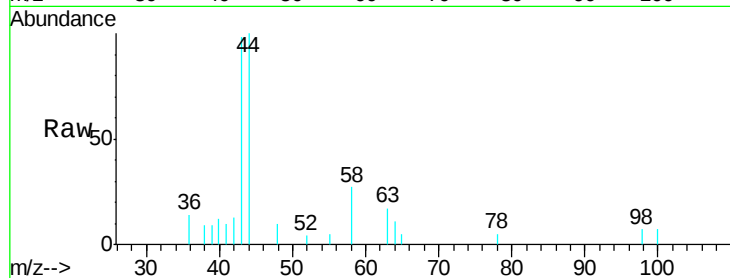



Abundance Ion 43.05 (42.75 to 43.75): VU035151.D (-362) (-)

Ion 58.05 (57.75 to 58.75): VU035151.D (-362) (-)

2.31

2.35

Time-->

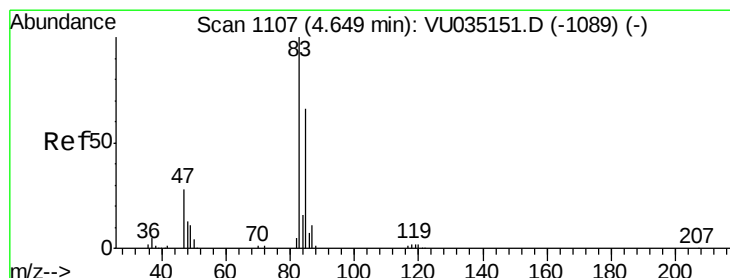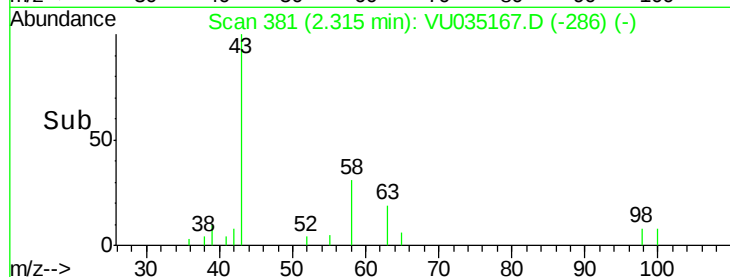

#25

Chloroform

Concen: 0.574 ug/L

RT: 4.65 min Scan# 1107

Delta R.T. -0.00 min

Lab File: VU035167.D


Acq: 14 Oct 2019 22:14

Tgt Ion: 83 Resp: 12264

Ion Ratio Lower Upper

83 100

85 69.3 45.4 84.4

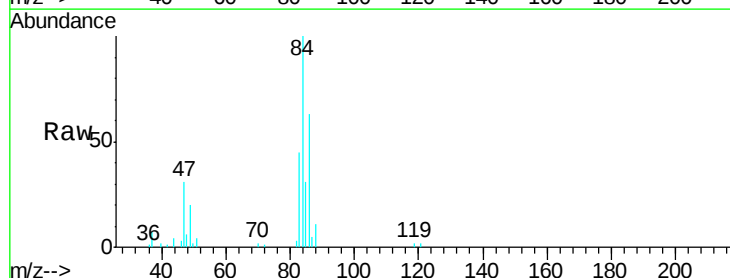


Abundance Ion 83.05 (82.75 to 83.75): VU035151.D (-1089) (-)


Ion 85.00 (84.70 to 85.70): VU035151.D (-1089) (-)

4.65

4.70

Time-->

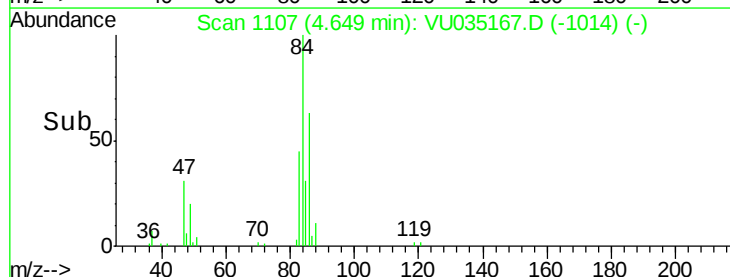

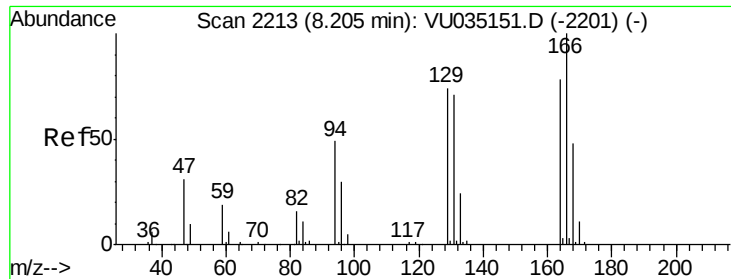

#47

Tetrachloroethene

Concen: 0.519 ug/L

RT: 8.21 min Scan# 2215

Delta R.T. 0.01 min

Lab File: VU035167.D


Acq: 14 Oct 2019 22:14

Instrument :

MSVOA_U

ClientSampleId :

C0CE4

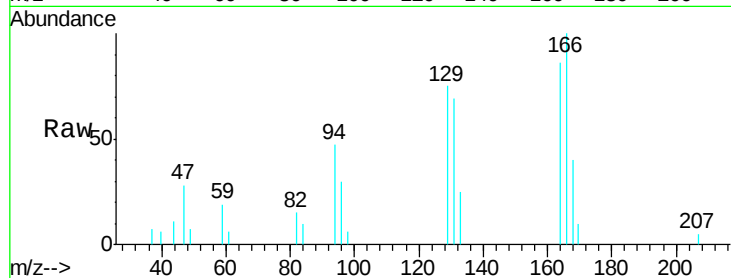

Tgt Ion:164 Resp: 4839

Ion Ratio Lower Upper

164 100

129 87.3 68.5 127.1

131 80.9 67.3 124.9

166 116.4 93.1 172.9

