

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101419\
 Data File : VU035163.D
 Acq On : 14 Oct 2019 20:36
 Operator : JC/SP
 Sample : K5311-06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 P0002-STEELE-191007-02

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.206	29	36	56	rVB	644609	675592	100.00%	12.000%
2	1.396	88	95	107	rBV	66949	70105	10.38%	1.245%
3	1.675	173	182	194	rBV	62320	80365	11.90%	1.427%
4	2.264	354	365	375	rBV	103991	160375	23.74%	2.849%
5	2.984	578	589	604	rVB6	9111	22396	3.32%	0.398%
6	4.196	945	966	993	rBV2	105978	430340	63.70%	7.644%
7	4.627	1083	1100	1125	rBV2	78422	216164	32.00%	3.839%
8	5.315	1292	1314	1338	rBV3	167337	475618	70.40%	8.448%
9	5.865	1472	1485	1507	rBV	166168	341228	50.51%	6.061%
10	6.167	1565	1579	1598	rBV	103898	214576	31.76%	3.811%
11	6.312	1610	1624	1650	rBV	119443	245968	36.41%	4.369%
12	7.212	1889	1904	1937	rBV	44889	96139	14.23%	1.708%
13	7.546	1995	2008	2032	rBV	188837	354590	52.49%	6.298%
14	7.836	2088	2098	2125	rBV	25267	55022	8.14%	0.977%
15	8.206	2201	2213	2232	rBV	188543	335174	49.61%	5.953%
16	8.305	2232	2244	2289	rVV	188591	574970	85.11%	10.212%
17	9.070	2469	2482	2519	rBV	237478	464935	68.82%	8.258%
18	10.414	2888	2900	2927	rBV	99859	175668	26.00%	3.120%
19	11.469	3216	3228	3262	rBV	165192	339809	50.30%	6.036%
20	11.845	3332	3345	3368	rBV2	156373	301057	44.56%	5.347%


Sum of corrected areas: 5630091

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU101419\
Data File : VU035163.D
Acq On : 14 Oct 2019 20:36
Operator : JC/SP
Sample : K5311-06
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
P0002-STEELE-191007-02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

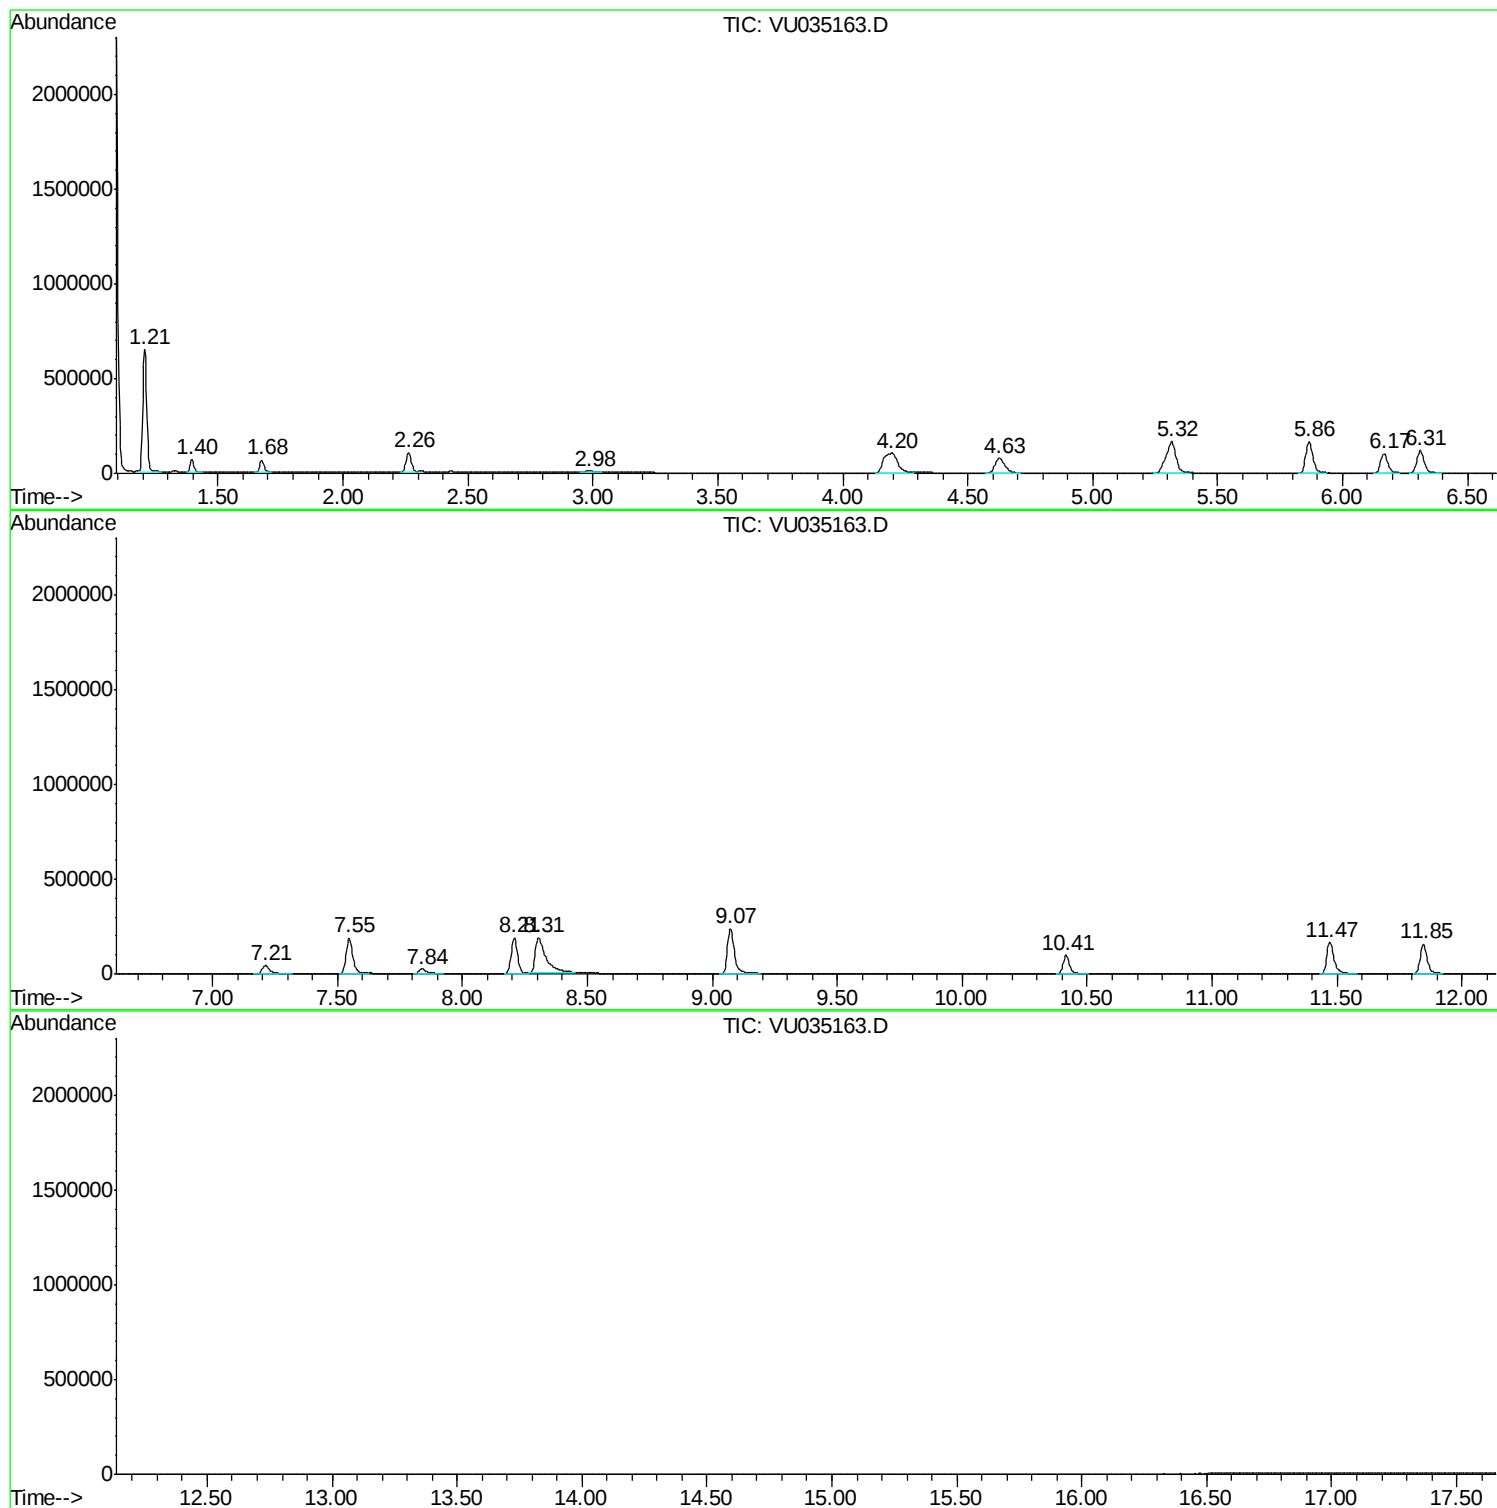

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101419\
Data File : VU035163.D
Acq On : 14 Oct 2019 20:36
Operator : JC/SP
Sample : K5311-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
P0002-STEELE-191007-02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101419\
Data File : VU035163.D
Acq On : 14 Oct 2019 20:36
Operator : JC/SP
Sample : K5311-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
P0002-STEELE-191007-02

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc