


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU101419\
Data File : VU035139.D
Acq On : 14 Oct 2019 09:35
Operator : JC/SP
Sample : BFB19
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB19

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Oct 16 05:10:52 2019

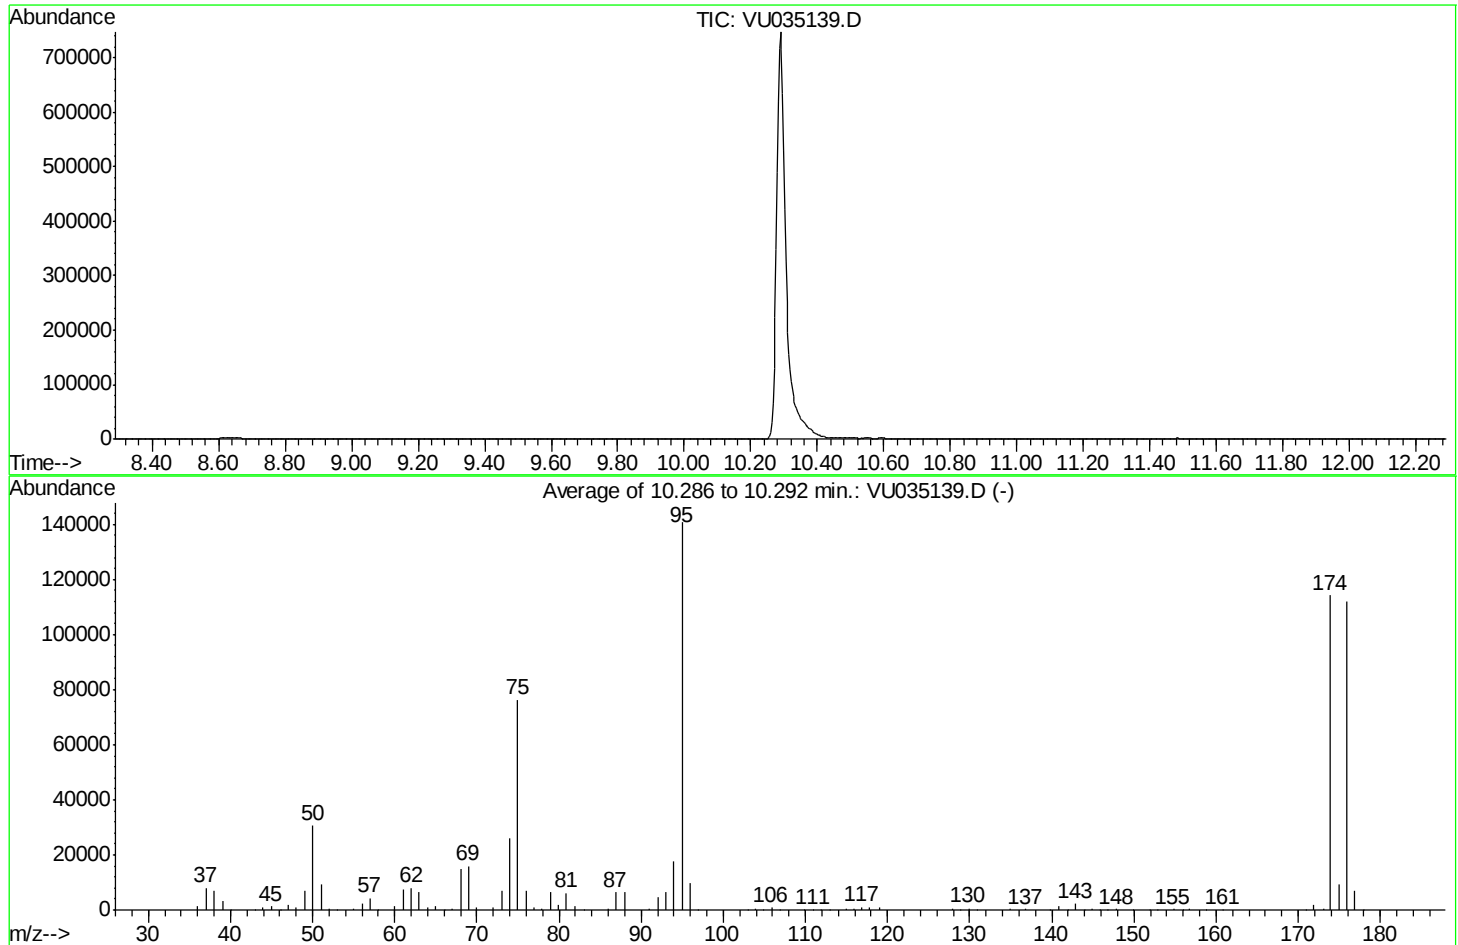

AutoFind: Scans 2860, 2861, 2862; Background Corrected with Scan 2847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	30624	PASS
75	95	30	80	54.2	76269	PASS
95	95	100	100	100.0	140757	PASS
96	95	5	9	6.9	9742	PASS
173	174	0.00	2	0.6	697	PASS
174	95	50	120	81.1	114216	PASS
175	174	5	9	8.2	9416	PASS
176	174	95	101	97.9	111856	PASS
177	176	5	9	6.2	6971	PASS

Scan 2847 (10.244 min): VU035139.D
BFB19

m/z	Abundance
40.00	157.0
43.90	468.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

m/z	Abundance
36.00	1452.0
37.00	8253.0
38.00	6999.0
39.00	3315.0
40.00	276.0
43.00	124.0
44.00	1474.0
45.00	1312.0
46.00	220.0
47.00	1521.0
48.00	1141.0
49.00	6826.0
50.00	30568.0
51.00	9362.0
52.00	394.0
52.90	128.0
54.90	506.0
56.00	2548.0
57.00	4388.0
57.90	242.0
60.00	1551.0
61.00	7584.0
62.00	8012.0
63.00	6556.0
64.00	811.0
65.00	1406.0
66.00	198.0
66.90	353.0
68.00	14662.0
69.00	15978.0
70.00	1144.0
72.00	743.0
73.00	6971.0
74.00	25720.0
75.00	75280.0
76.00	6673.0
77.00	945.0
78.00	727.0
78.90	6512.0
80.00	1735.0
80.90	5959.0
81.90	1393.0
83.00	102.0
86.10	278.0
86.90	6441.0
87.90	6164.0
90.90	575.0
92.00	4382.0
93.00	6502.0
94.00	17616.0
95.00	138688.0
96.00	9874.0
96.90	226.0
104.00	725.0
104.90	147.0
105.90	739.0
106.80	135.0
109.80	102.0
110.90	186.0
111.80	101.0
112.90	131.0
114.90	246.0
115.90	516.0
116.90	1097.0
117.80	693.0
119.00	983.0
127.90	562.0
128.90	196.0
129.90	596.0
130.90	225.0
134.90	276.0
136.90	354.0
140.90	1548.0
141.90	161.0
142.90	2313.0
144.00	163.0
144.90	412.0
145.80	168.0
147.90	271.0
149.80	162.0
151.80	110.0
152.80	159.0
154.80	340.0
156.00	113.0
156.80	247.0
158.80	240.0
160.80	129.0
170.90	225.0
171.90	1791.0
173.10	2092.0
173.90	110352.0
175.00	9126.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

175.90	108480.0
176.90	6813.0
177.90	236.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

m/z	Abundance
36.00	1470.0
37.00	8126.0
38.00	7119.0
39.00	3234.0
40.00	306.0
43.00	135.0
44.00	1385.0
45.00	1370.0
46.10	179.0
47.10	1706.0
48.00	1180.0
49.00	7051.0
50.00	31576.0
51.10	9555.0
52.00	405.0
52.90	135.0
55.00	516.0
56.00	2601.0
57.00	4452.0
58.00	205.0
60.00	1624.0
61.00	7907.0
62.00	8150.0
63.00	6691.0
64.00	774.0
65.00	1498.0
66.00	185.0
66.90	354.0
68.00	15423.0
69.00	16512.0
70.00	1131.0
72.00	761.0
73.00	7346.0
74.00	26648.0
75.00	78408.0
76.00	7068.0
77.00	1027.0
77.90	731.0
78.90	6503.0
80.00	1764.0
80.90	6336.0
81.90	1522.0
83.10	133.0
86.10	259.0
86.90	6588.0
87.90	6541.0
90.90	646.0
92.00	4629.0
93.00	6913.0
94.00	18424.0
95.00	145024.0
96.00	9998.0
96.90	242.0
104.00	744.0
104.90	203.0
105.90	796.0
106.80	163.0
110.90	160.0
111.80	113.0
112.90	104.0
114.90	309.0
115.80	515.0
116.90	1070.0
117.90	760.0
119.00	1020.0
127.90	532.0
128.90	216.0
129.90	697.0
130.80	232.0
134.90	307.0
136.90	327.0
139.80	109.0
140.90	1544.0
141.90	199.0
142.90	2391.0
144.00	180.0
144.80	425.0
145.80	129.0
147.90	279.0
149.80	164.0
151.90	120.0
152.80	178.0
154.90	372.0
156.00	149.0
156.80	265.0
158.70	186.0
160.90	149.0
170.90	223.0
171.90	1870.0
173.90	117592.0
175.00	9815.0
175.90	115216.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

176.907147.0

177.90266.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

m/z	Abundance
36.00	1354.0
37.00	7401.0
38.00	6721.0
39.10	2869.0
40.00	315.0
43.00	135.0
44.00	1251.0
45.00	1315.0
46.10	159.0
47.00	1720.0
48.00	1101.0
49.00	6553.0
50.00	29728.0
51.10	8859.0
52.00	383.0
52.90	135.0
55.00	440.0
56.00	2462.0
57.00	4189.0
58.00	146.0
60.00	1524.0
61.00	7427.0
62.00	7617.0
63.00	6315.0
64.00	700.0
65.00	1466.0
66.00	145.0
66.90	338.0
68.00	14940.0
69.00	15394.0
70.00	1103.0
72.00	734.0
73.00	7239.0
74.00	25584.0
75.00	75120.0
76.00	6713.0
77.00	959.0
77.90	651.0
78.90	5904.0
79.90	1681.0
80.90	6123.0
81.90	1387.0
83.10	151.0
85.90	270.0
86.90	6062.0
88.00	6281.0
90.90	685.0
92.00	4443.0
93.00	6696.0
94.00	17528.0
95.00	138560.0
96.00	9356.0
97.00	248.0
102.90	146.0
103.90	666.0
104.90	249.0
105.90	742.0
106.90	162.0
111.00	170.0
111.90	134.0
114.90	292.0
115.80	469.0
116.80	986.0
117.90	719.0
119.00	917.0
127.90	463.0
128.90	216.0
129.90	705.0
130.80	214.0
134.90	338.0
136.80	273.0
139.80	139.0
140.90	1439.0
141.90	203.0
142.90	2167.0
144.00	154.0
144.90	451.0
145.90	124.0
146.80	112.0
147.90	311.0
149.80	141.0
152.80	152.0
154.90	339.0
156.00	165.0
156.80	270.0
158.70	128.0
160.90	139.0
170.90	189.0
171.90	1761.0
173.90	114704.0
175.00	9309.0
175.90	111872.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

176.90	6953.0
177.90	234.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19