


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU101420\
Data File : VU040690.D
Acq On : 14 Oct 2020 10:07
Operator : SY/MD
Sample : BFB20
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB20

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Oct 15 05:23:17 2020

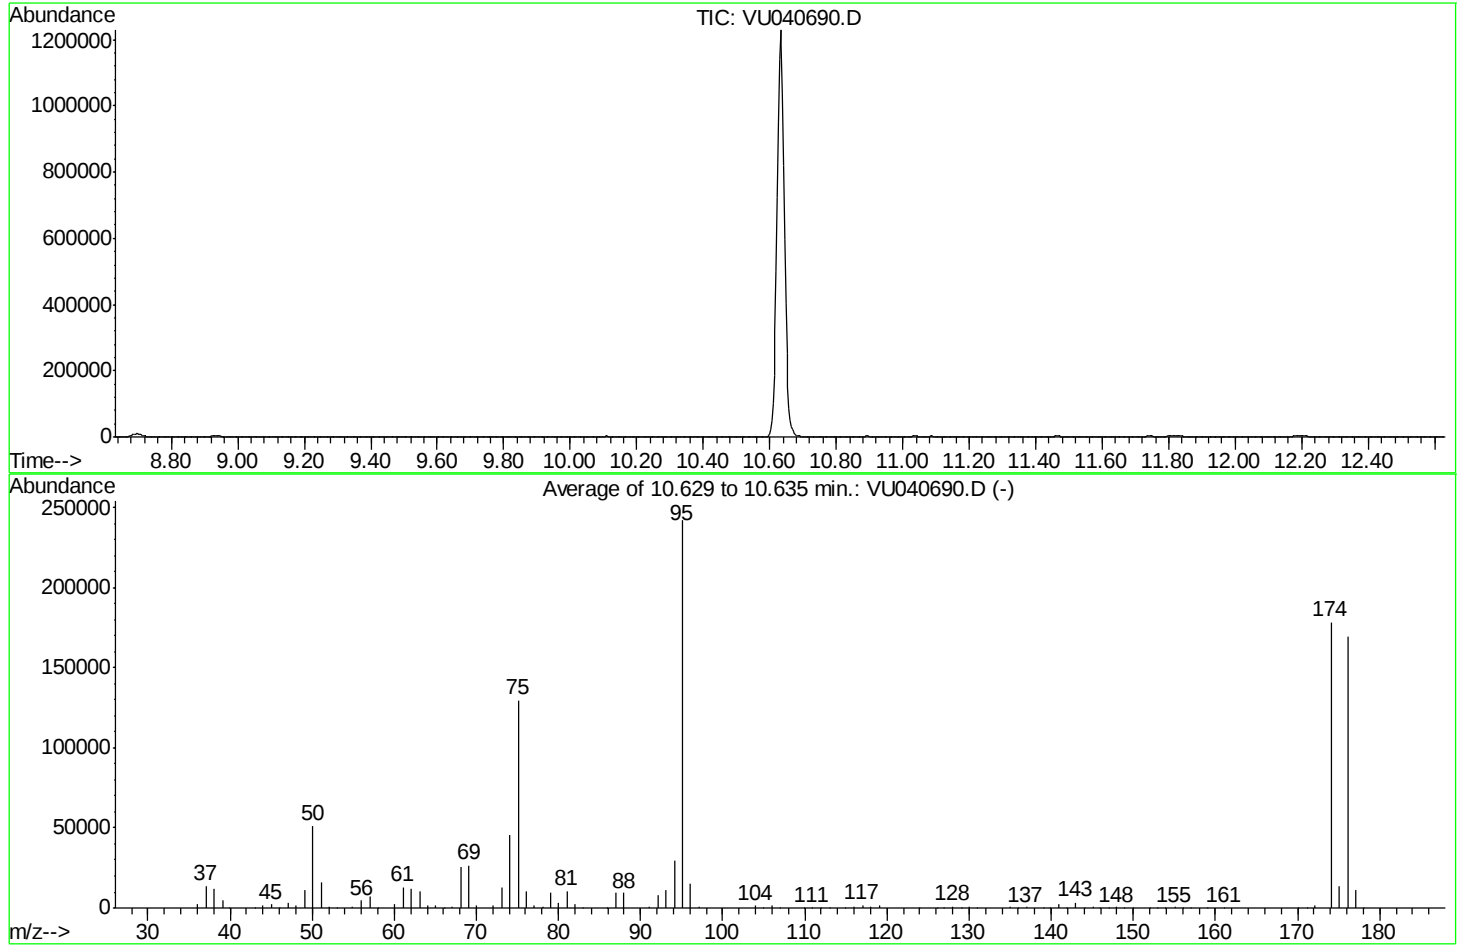

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	51496	PASS
75	95	30	80	53.6	129650	PASS
95	95	100	100	100.0	242048	PASS
96	95	5	9	6.2	15124	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.8	178517	PASS
175	174	5	9	7.5	13446	PASS
176	174	95	101	95.1	169685	PASS
177	176	5	9	6.4	10855	PASS

m/z	Abundance
36.00	2371.0
37.10	13452.0
38.00	12166.0
39.10	4748.0
40.00	276.0
43.00	129.0
44.00	1826.0
45.00	2256.0
46.00	280.0
47.10	3215.0
48.10	1645.0
49.10	11015.0
50.10	50112.0
51.10	15920.0
52.10	593.0
53.00	174.0
55.00	702.0
56.00	4302.0
57.10	7014.0
58.00	375.0
60.00	2547.0
61.10	13081.0
62.10	12319.0
63.10	10332.0
64.00	1255.0
65.00	1586.0
66.10	251.0
67.10	813.0
68.10	25344.0
69.10	25768.0
70.00	1832.0
72.00	1062.0
73.10	12512.0
74.10	43960.0
75.10	125944.0
76.10	10310.0
77.10	1378.0
78.10	1126.0
79.00	9631.0
80.00	2641.0
81.00	10454.0
82.00	2118.0
83.00	231.0
85.90	240.0
87.00	8593.0
88.00	8918.0
91.00	1188.0
92.10	7313.0
93.10	10991.0
94.10	28312.0
95.10	234048.0
96.10	14928.0
97.10	482.0
104.00	1363.0
104.90	323.0
106.00	1384.0
107.00	230.0
109.90	137.0
110.90	309.0
111.90	231.0
113.10	366.0
114.80	236.0
116.00	911.0
117.00	1789.0
118.00	948.0
119.00	1543.0
123.90	180.0
126.10	140.0
128.00	766.0
129.00	487.0
130.00	824.0
130.90	245.0
135.00	449.0
136.00	118.0
137.00	574.0
139.10	117.0
139.90	200.0
141.00	2570.0
141.90	271.0
143.00	3070.0
144.00	232.0
145.10	555.0
146.00	417.0
147.00	166.0
148.00	583.0
149.90	280.0
152.00	156.0
153.00	218.0
153.90	114.0
155.10	457.0
156.90	287.0
159.00	259.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20

161.00	250.0
170.10	115.0
171.10	405.0
172.10	1811.0
174.10	168128.0
175.10	13230.0
176.10	158016.0
177.10	10586.0
178.00	263.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20

m/z	Abundance
36.00	2637.0
37.10	14262.0
38.10	12779.0
39.10	4864.0
40.00	284.0
43.00	107.0
44.00	1819.0
45.00	2460.0
46.00	211.0
47.10	3381.0
48.10	1620.0
49.10	11659.0
50.10	53344.0
51.10	16672.0
52.10	644.0
53.00	192.0
54.90	681.0
56.00	4686.0
57.10	7397.0
58.00	431.0
60.10	2653.0
61.10	13439.0
62.10	12799.0
63.10	10415.0
64.00	1296.0
65.00	1495.0
66.10	196.0
67.10	885.0
68.10	26800.0
69.10	27328.0
70.10	1978.0
72.00	1306.0
73.10	13007.0
74.10	46688.0
75.10	134400.0
76.10	10871.0
77.00	1528.0
78.10	1331.0
79.00	9973.0
80.00	2964.0
81.00	11007.0
82.00	2291.0
83.00	303.0
85.90	279.0
87.00	9789.0
88.00	9813.0
91.00	1231.0
92.10	7923.0
93.10	12124.0
94.10	30816.0
95.10	251008.0
96.10	15576.0
97.10	450.0
104.00	1539.0
104.90	406.0
106.00	1402.0
107.00	257.0
109.90	157.0
110.90	285.0
112.00	173.0
113.10	419.0
114.90	277.0
116.00	1043.0
117.00	1951.0
118.00	1127.0
119.00	1571.0
123.90	161.0
126.10	142.0
128.00	914.0
129.00	438.0
130.00	848.0
131.00	297.0
135.00	538.0
136.00	115.0
137.00	592.0
139.10	100.0
139.90	247.0
141.00	2892.0
141.90	311.0
143.00	3351.0
144.00	246.0
145.10	591.0
146.00	415.0
147.00	156.0
148.00	661.0
148.90	109.0
149.90	253.0
152.00	141.0
153.00	231.0
153.90	113.0
155.00	501.0
157.00	408.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20

159.00	330.0
161.10	284.0
170.10	139.0
171.10	424.0
172.10	1844.0
174.10	184896.0
175.10	13911.0
176.10	176256.0
177.10	11185.0
178.00	312.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20

m/z	Abundance
36.10	2633.0
37.10	13454.0
38.10	12037.0
39.10	4500.0
39.90	290.0
44.10	1755.0
45.00	2362.0
46.00	171.0
47.10	3074.0
48.00	1389.0
49.10	10985.0
50.10	51032.0
51.10	15707.0
52.10	601.0
53.00	225.0
54.90	625.0
56.00	4458.0
57.10	6895.0
58.00	390.0
60.10	2439.0
61.00	12394.0
62.00	11929.0
63.10	9795.0
64.00	1192.0
65.00	1294.0
66.00	145.0
67.10	826.0
68.10	25680.0
69.10	26136.0
70.10	2007.0
72.00	1500.0
73.10	12120.0
74.10	45008.0
75.10	128608.0
76.10	10477.0
77.00	1542.0
78.10	1192.0
79.00	9471.0
80.00	3034.0
81.00	10517.0
82.00	2212.0
83.00	366.0
85.90	317.0
87.00	9696.0
88.00	9733.0
91.00	1196.0
92.10	7739.0
93.10	11441.0
94.10	30656.0
95.10	241088.0
96.10	14870.0
97.10	443.0
104.00	1464.0
104.90	443.0
106.00	1267.0
107.00	229.0
109.90	161.0
110.90	224.0
112.00	142.0
113.00	341.0
114.90	304.0
116.00	1080.0
117.00	1927.0
118.00	1183.0
119.10	1506.0
124.00	129.0
126.90	111.0
128.00	931.0
129.10	365.0
130.00	828.0
131.00	348.0
135.00	519.0
137.00	525.0
139.90	245.0
141.00	2898.0
141.90	311.0
143.00	3203.0
144.00	205.0
145.10	557.0
145.90	372.0
147.00	105.0
148.00	633.0
148.90	145.0
149.90	206.0
151.90	125.0
152.90	189.0
155.00	562.0
156.10	106.0
157.00	528.0
159.00	369.0
161.00	304.0
170.10	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20

171.10	381.0
172.10	1622.0
174.10	182528.0
175.10	13199.0
176.10	174784.0
177.10	10795.0
178.00	315.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20

Scan 2875 (10.584 min): VU040690.D
BFB20

m/z	Abundance
39.90	103.0
44.00	261.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20