

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101422\
 Data File : VU051421.D
 Acq On : 14 Oct 2022 12:51
 Operator : JC/MD
 Sample : VU1014WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1014WBL01

Quant Time: Oct 15 06:08:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U100422DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Wed Oct 05 02:45:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.112	96	47753	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.632	95	11723	0.747	ug/l	0.00
Spiked Amount 1.000			Recovery	=	75.000%	
68) 1,2-Dichlorobenzene-d4	12.192	152	12409	0.711	ug/l	0.00
Spiked Amount 1.000			Recovery	=	71.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101422\
Data File : VU051421.D
Acq On : 14 Oct 2022 12:51
Operator : JC/MD
Sample : VU1014WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1014WBL01

Quant Time: Oct 15 06:08:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U100422DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Wed Oct 05 02:45:21 2022
Response via : Initial Calibration




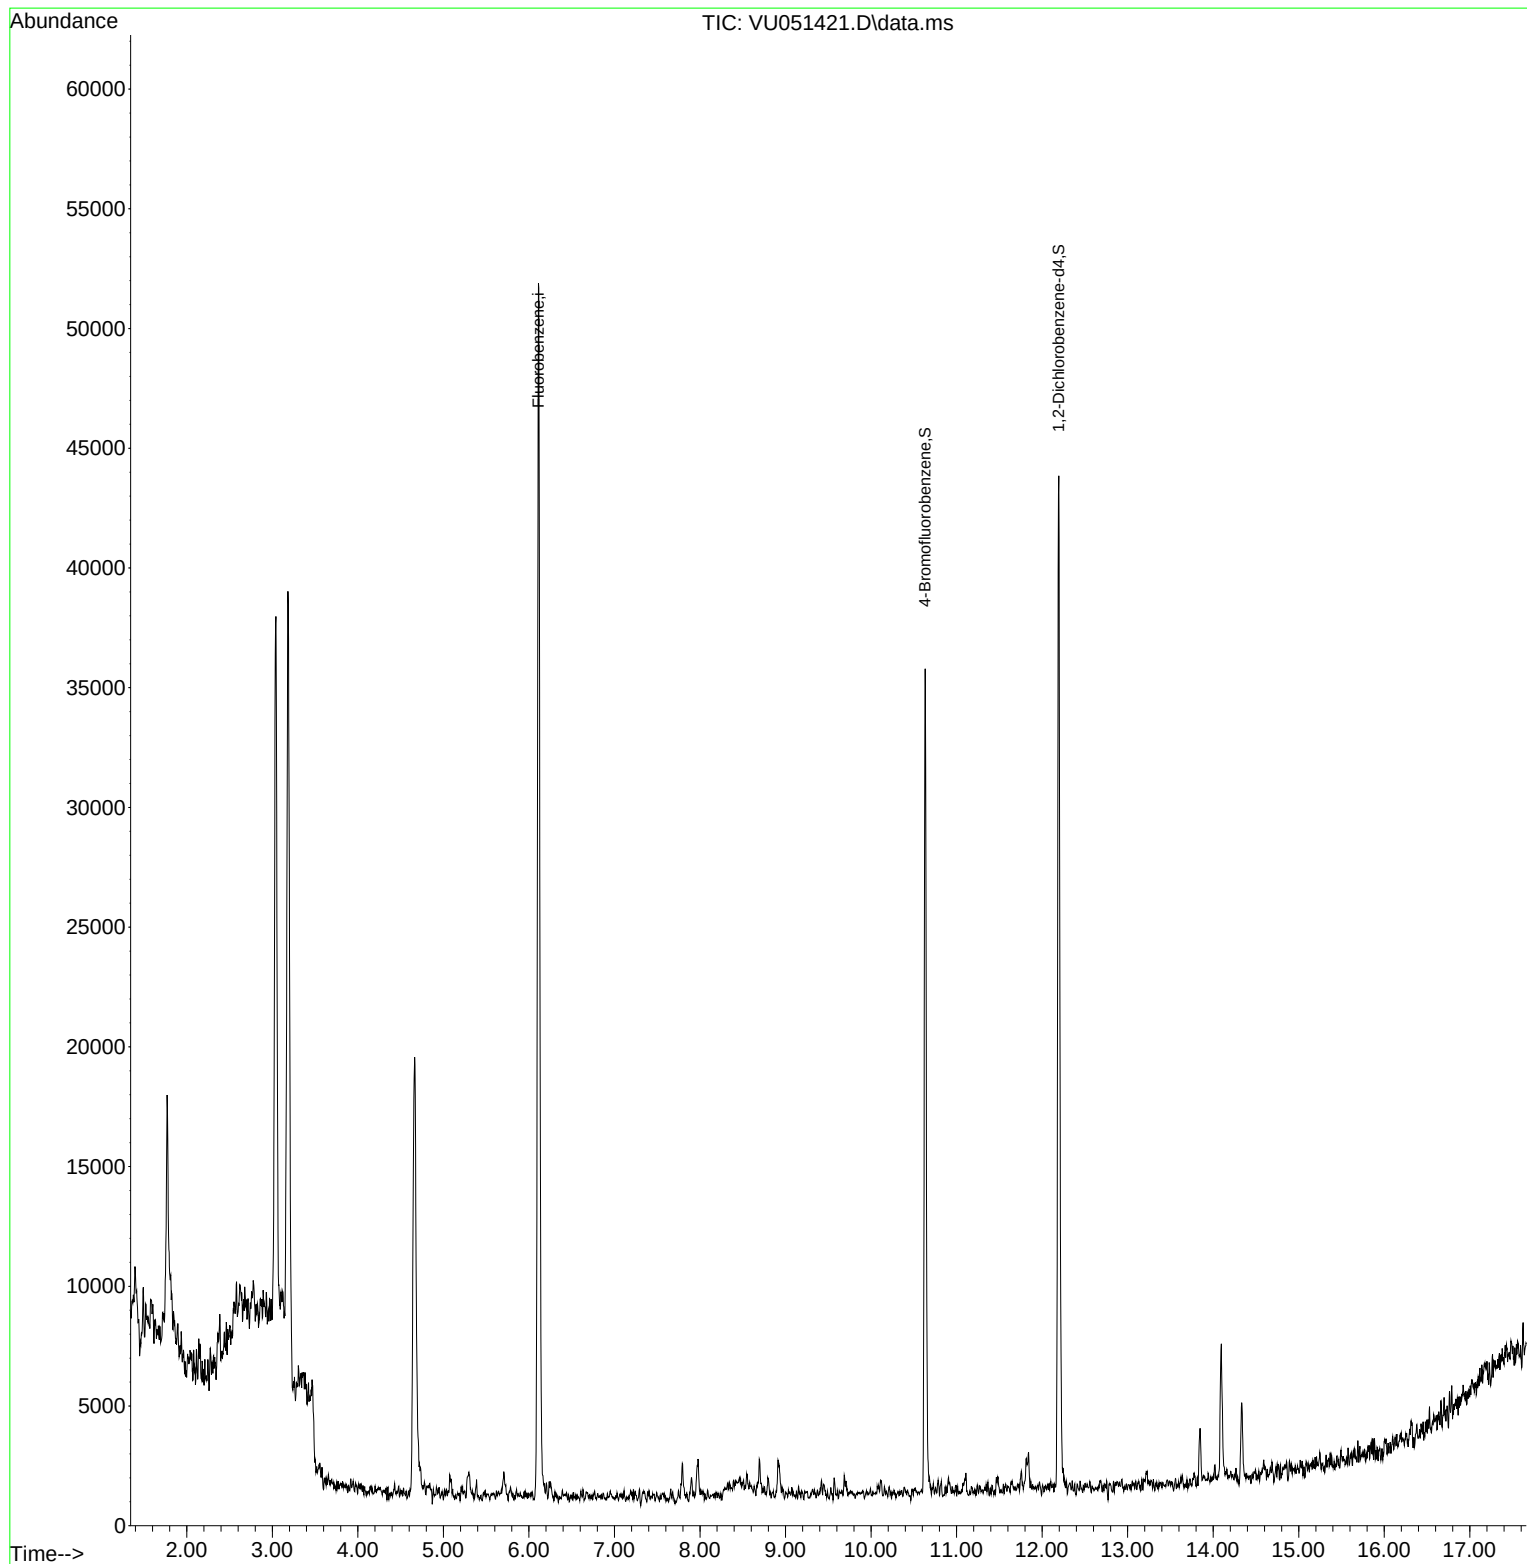


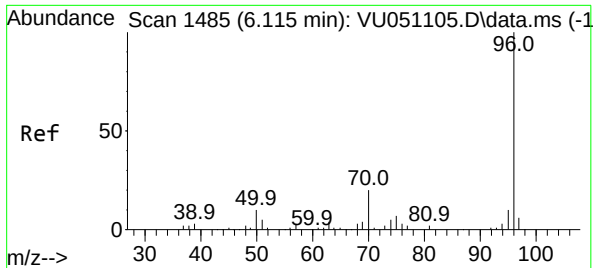

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.112 min Scan# 1485
Delta R.T. -0.003 min
Lab File: VU051421.D
Acq: 14 Oct 2022 12:51




Instrument :
MSVOA_U
ClientSampleId :
VU1014WBL01


Tgt Ion: 96 Resp: 47753
Ion Ratio Lower Upper
96 100
70 19.9 16.7 25.1
95 8.4 7.4 11.0
97 5.6 0.0 0.0#

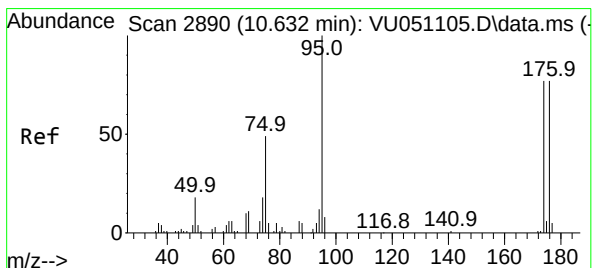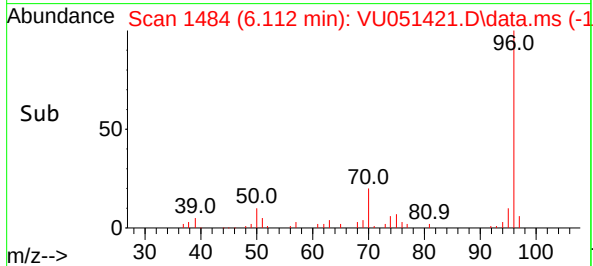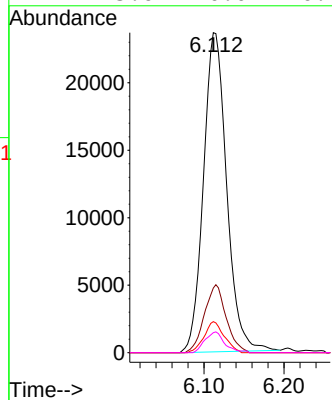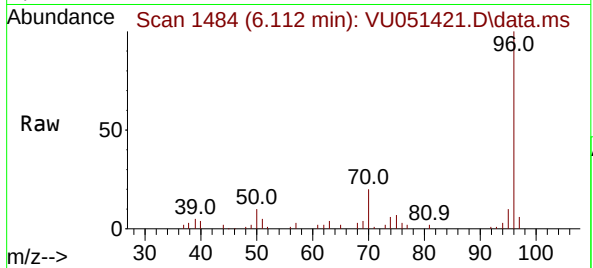

#57
4-Bromofluorobenzene
Concen: 0.747 ug/l
RT: 10.632 min Scan# 2890
Delta R.T. -0.000 min
Lab File: VU051421.D
Acq: 14 Oct 2022 12:51

Tgt Ion: 95 Resp: 11723
Ion Ratio Lower Upper
95 100
174 79.9 62.4 93.6
176 79.1 56.2 84.2

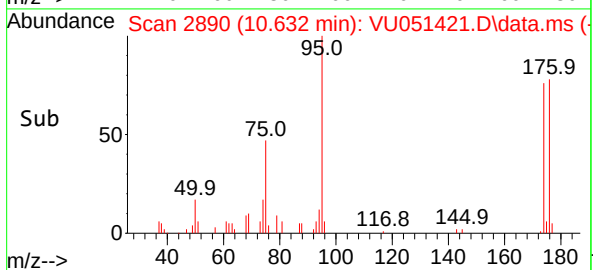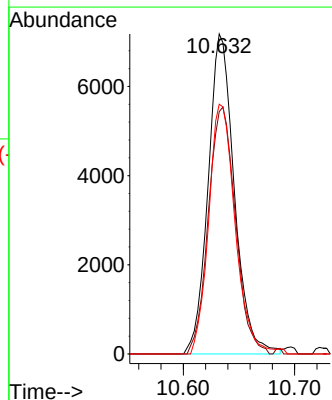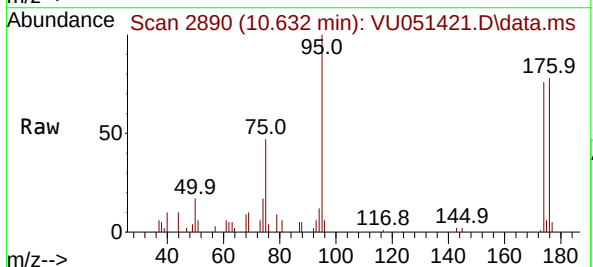

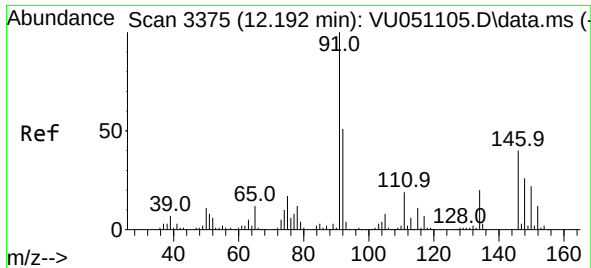

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.711 ug/l
 RT: 12.192 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VU051421.D
 Acq: 14 Oct 2022 12:51

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1014WBL01

Tgt Ion	Ratio	Lower	Upper
152	100		
115	65.3	0.0	254.6
150	153.3	0.0	623.6

