

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101422\
 Data File : VU051424.D
 Acq On : 14 Oct 2022 15:15
 Operator : JC/MD
 Sample : N4817-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 38025-110221

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U100422DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU051424.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.041	519	529	540	rVB	28955	50953	2.07%	1.006%
2	3.182	562	573	590	rVB	45931	109154	4.43%	2.154%
3	4.661	1017	1033	1051	rBV	21883	53406	2.17%	1.054%
4	5.086	1147	1165	1194	rBV	464748	1000308	40.58%	19.742%
5	6.111	1471	1484	1507	rBV	51190	101322	4.11%	2.000%
6	7.105	1776	1793	1815	rBV	1360865	2465089	100.00%	48.652%
7	8.809	2309	2323	2348	rBV	488531	847426	34.38%	16.725%
8	10.288	2771	2783	2801	rBV	178992	309274	12.55%	6.104%
9	10.632	2881	2890	2905	rBV2	34855	57260	2.32%	1.130%
10	12.192	3365	3375	3391	rBV2	43279	72617	2.95%	1.433%




Sum of corrected areas: 5066809

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU01422\
Data File : VU051424.D
Acq On : 14 Oct 2022 15:15
Operator : JC/MD
Sample : N4817-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
38025-110221

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U100422DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

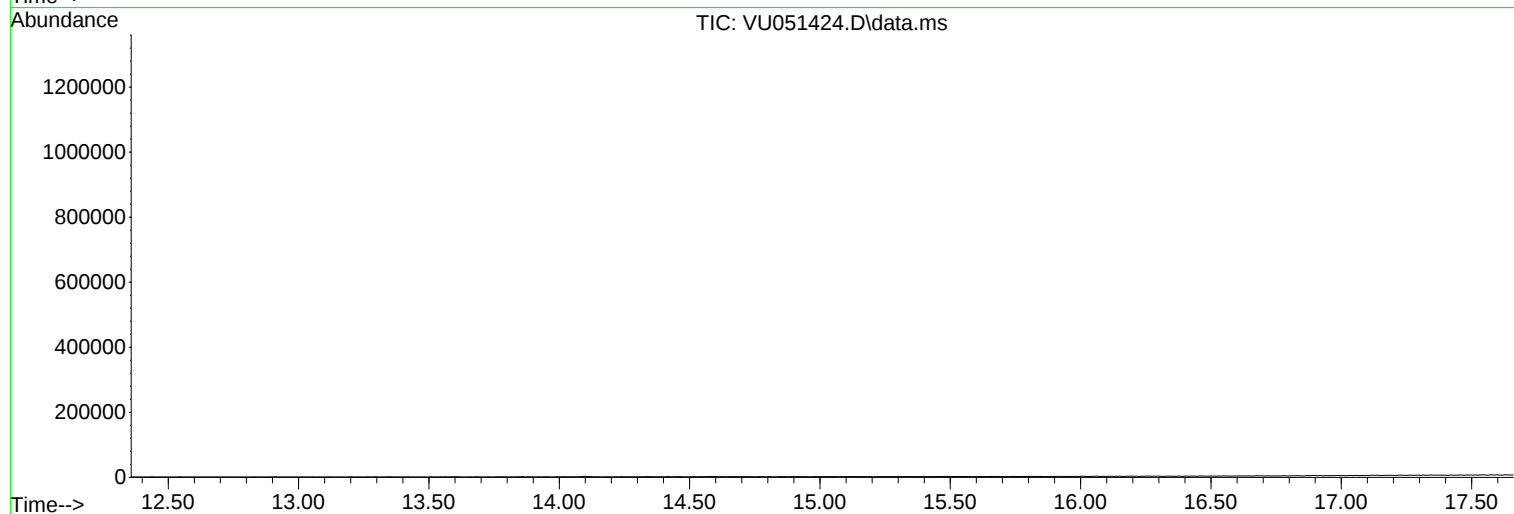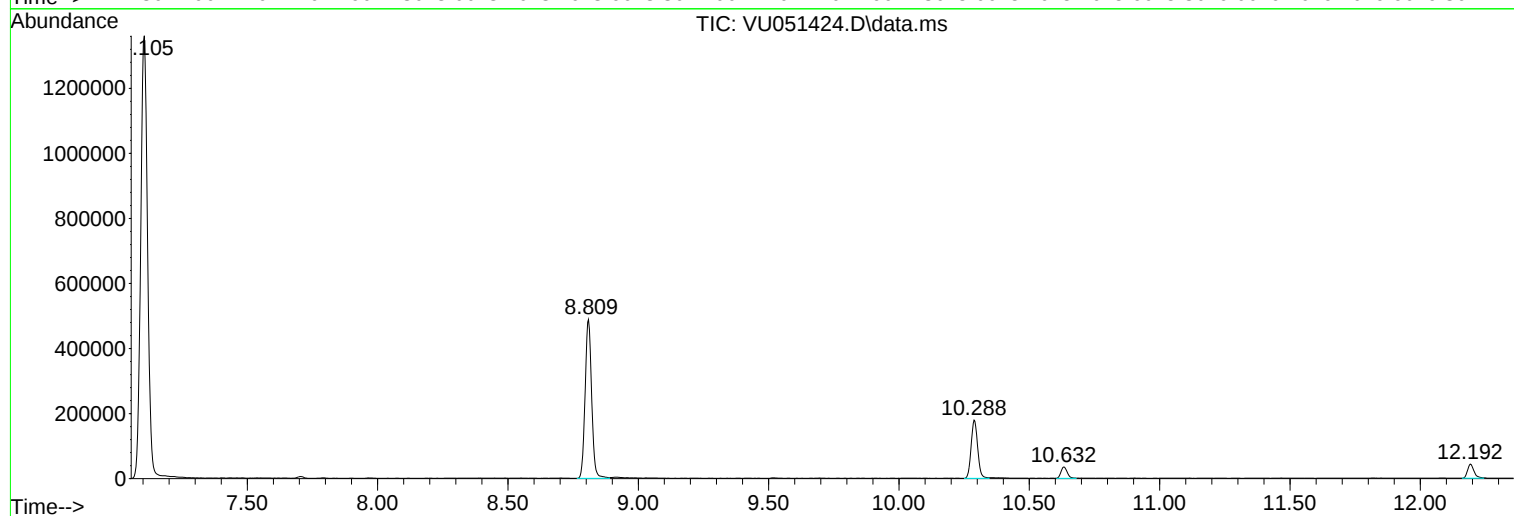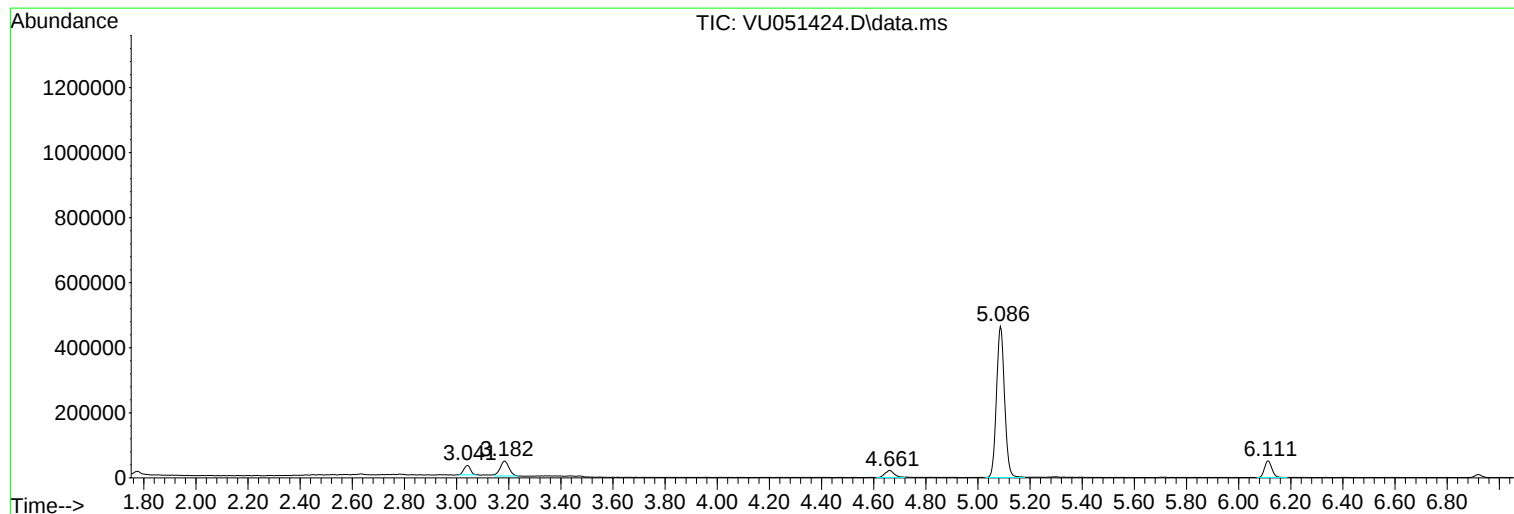

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101422\
Data File : VU051424.D
Acq On : 14 Oct 2022 15:15
Operator : JC/MD
Sample : N4817-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
38025-110221

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U100422DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101422\
Data File : VU051424.D
Acq On : 14 Oct 2022 15:15
Operator : JC/MD
Sample : N4817-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
38025-110221

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U100422DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------