
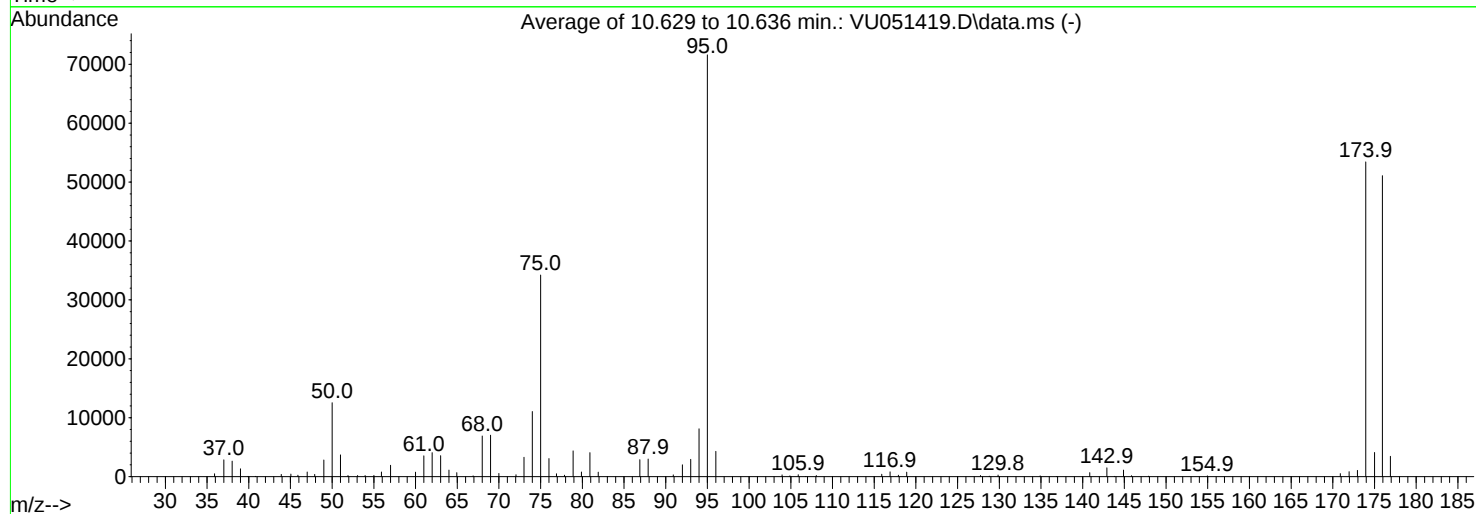


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU101422\  
 Data File : VU051419.D  
 Acq On : 14 Oct 2022 11:20  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\524U100422DW.M  
 Title : METHOD 524.2 VOLATILES DRINKING WATER  
 Last Update : Wed Oct 05 02:45:21 2022

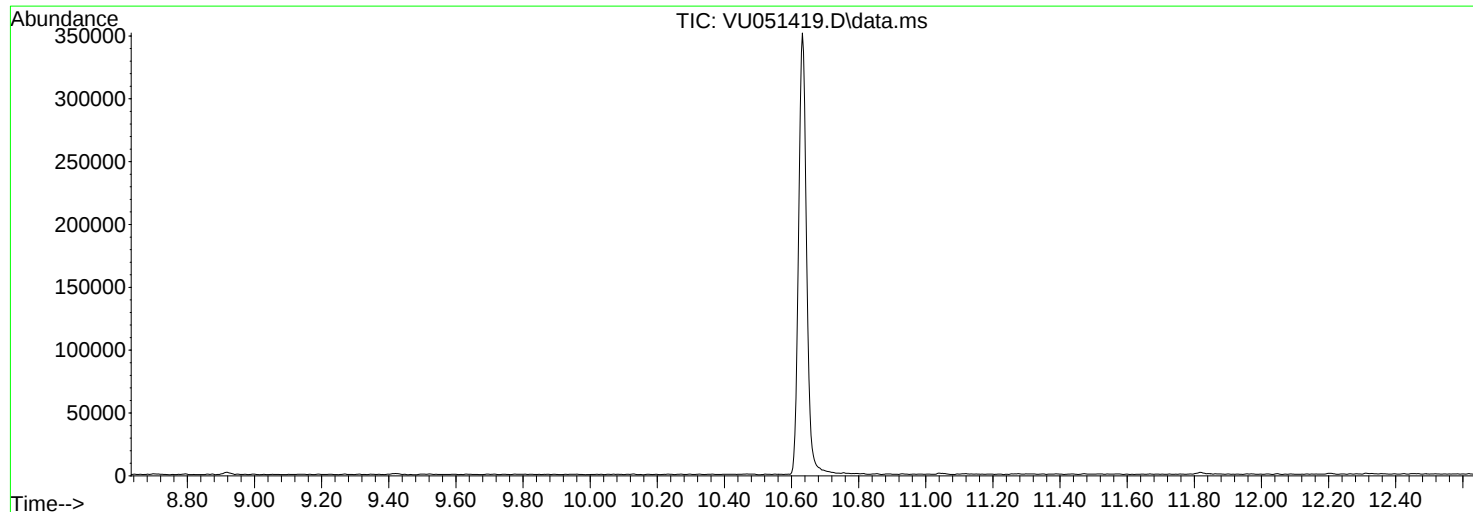

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 17.5         | 12547      | PASS                |
| 75             | 95              | 30              | 60              | 47.8         | 34219      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 71600      | PASS                |
| 96             | 95              | 5               | 9               | 6.0          | 4307       | PASS                |
| 173            | 174             | 0.00            | 2               | 2.0          | 1049       | PASS                |
| 174            | 95              | 50              | 100             | 74.6         | 53435      | PASS                |
| 175            | 174             | 5               | 9               | 7.7          | 4114       | PASS                |
| 176            | 174             | 95              | 101             | 95.6         | 51077      | PASS                |
| 177            | 176             | 5               | 9               | 6.7          | 3445       | PASS                |