


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101424\
Data File : VU061125.D
Acq On : 14 Oct 2024 08:57
Operator : MD/SY
Sample : BFB012
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB012

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Oct 15 05:36:38 2024

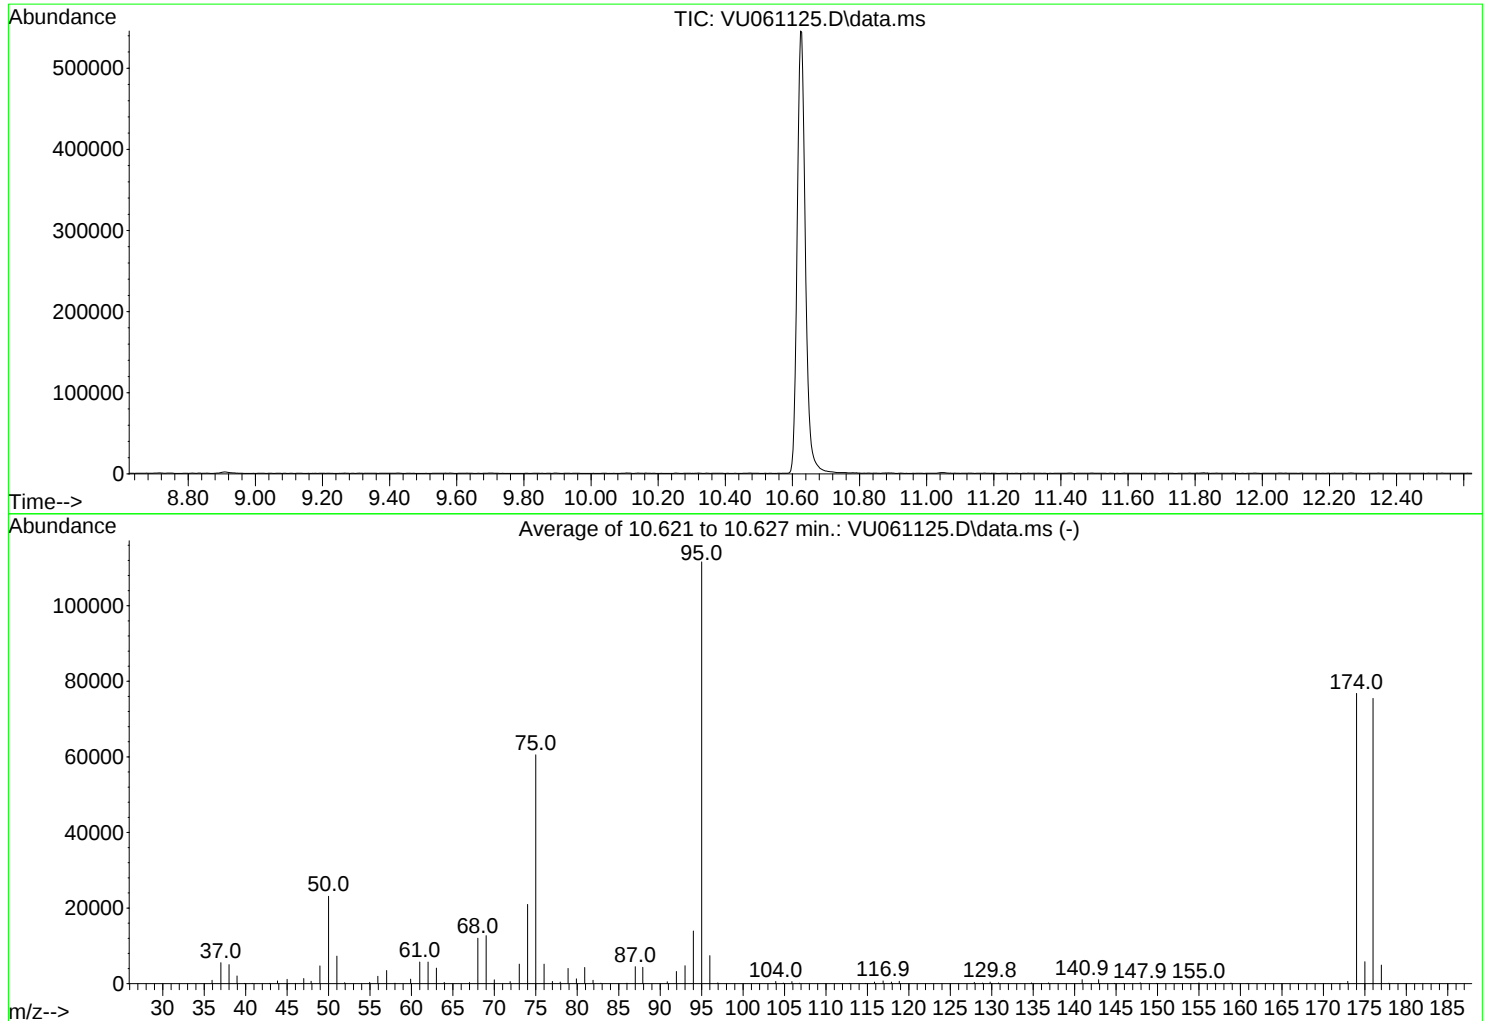

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2889

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.7	23109	PASS
75	95	30	80	54.2	60539	PASS
95	95	100	100	100.0	111611	PASS
96	95	5	9	6.6	7395	PASS
173	174	0.00	2	0.8	590	PASS
174	95	50	120	68.8	76797	PASS
175	174	5	9	7.5	5791	PASS
176	174	95	101	98.3	75475	PASS
177	176	5	9	6.5	4917	PASS

m/z	Abundance
39.80	318.0
43.80	390.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012

m/z	Abundance
36.00	927.0
37.00	5306.0
38.00	4712.0
39.00	1951.0
39.90	398.0
43.90	1143.0
45.00	1104.0
46.00	106.0
47.00	1237.0
47.90	553.0
49.00	4663.0
50.00	22032.0
51.00	6995.0
52.00	262.0
55.00	350.0
55.90	1826.0
57.00	3330.0
58.00	135.0
59.90	1134.0
61.00	5310.0
62.00	5437.0
63.00	3972.0
63.90	320.0
67.00	310.0
68.00	11479.0
69.00	11932.0
70.00	984.0
71.90	489.0
73.00	5003.0
74.00	20064.0
75.00	57160.0
76.00	4863.0
77.00	570.0
77.90	410.0
78.90	3818.0
79.90	1151.0
80.90	3936.0
81.90	910.0
82.90	108.0
86.00	143.0
87.00	4325.0
87.90	4071.0
90.90	537.0
92.00	2990.0
93.00	4555.0
94.00	13234.0
95.00	105432.0
96.00	7201.0
97.00	188.0
103.90	521.0
104.90	184.0
105.90	513.0
106.80	101.0
115.80	406.0
116.90	651.0
117.90	403.0
118.90	604.0
127.90	295.0
128.90	171.0
129.80	379.0
130.80	197.0
134.80	198.0
136.80	204.0
140.90	1025.0
142.00	111.0
142.90	1036.0
144.80	122.0
147.90	207.0
155.00	230.0
156.90	125.0
158.90	149.0
172.90	564.0
174.00	71120.0
175.00	5449.0
176.00	69936.0
177.00	4773.0
177.90	116.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012

m/z	Abundance
35.90	921.0
37.00	5692.0
38.00	5218.0
39.00	2092.0
39.90	409.0
40.80	105.0
42.90	101.0
43.90	1150.0
45.00	1230.0
46.00	106.0
47.00	1417.0
47.90	660.0
49.00	4808.0
50.00	23880.0
51.00	7489.0
51.90	259.0
54.90	349.0
56.00	2015.0
57.00	3603.0
58.00	145.0
59.90	1206.0
61.00	5904.0
62.00	5883.0
63.00	4163.0
64.00	343.0
67.00	320.0
68.00	12375.0
69.00	13090.0
70.00	1030.0
71.90	546.0
73.00	5351.0
74.00	21512.0
75.00	62440.0
76.00	5305.0
77.00	609.0
77.90	438.0
78.90	4161.0
79.90	1352.0
80.90	4413.0
81.90	932.0
82.80	118.0
86.00	146.0
87.00	4650.0
87.90	4442.0
90.80	536.0
92.00	3365.0
93.00	4877.0
94.00	14394.0
95.00	114840.0
96.00	7650.0
96.90	221.0
104.00	610.0
104.80	193.0
105.90	557.0
106.80	125.0
112.80	102.0
114.80	112.0
115.80	420.0
116.90	723.0
117.90	462.0
118.90	629.0
127.90	335.0
128.90	170.0
129.80	469.0
130.80	225.0
134.80	220.0
136.90	210.0
140.90	1114.0
142.90	1114.0
144.80	107.0
145.90	121.0
147.90	237.0
149.90	132.0
155.00	224.0
156.90	136.0
158.90	166.0
160.80	120.0
172.90	588.0
174.00	79016.0
175.00	6013.0
176.00	77776.0
177.00	5038.0
177.90	135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012

m/z	Abundance
35.90	841.0
37.00	5606.0
38.00	5200.0
38.90	2080.0
39.90	357.0
40.80	104.0
42.90	104.0
43.90	1071.0
45.00	1154.0
47.00	1417.0
47.90	710.0
48.90	4625.0
50.00	23416.0
51.00	7405.0
51.90	223.0
54.90	331.0
56.00	1991.0
57.00	3433.0
58.00	154.0
59.90	1190.0
61.00	6002.0
62.00	5803.0
63.00	4150.0
64.00	358.0
67.00	313.0
68.00	12198.0
69.00	13052.0
70.00	1019.0
71.90	596.0
73.00	5204.0
74.00	21344.0
75.00	62016.0
76.00	5337.0
77.00	647.0
78.00	471.0
78.90	4163.0
79.90	1334.0
80.90	4528.0
81.90	891.0
82.90	105.0
86.00	134.0
87.00	4447.0
87.90	4438.0
90.80	501.0
91.90	3337.0
93.00	4794.0
94.00	14142.0
95.00	114560.0
96.00	7334.0
96.90	239.0
103.90	613.0
104.80	175.0
105.90	584.0
106.80	117.0
112.90	105.0
114.80	143.0
115.90	406.0
116.90	739.0
117.90	459.0
118.80	614.0
127.90	344.0
128.90	165.0
129.80	456.0
130.80	201.0
134.80	230.0
136.90	209.0
140.90	1102.0
142.90	1086.0
145.90	143.0
147.90	269.0
149.90	148.0
155.00	201.0
157.00	146.0
158.80	143.0
160.80	129.0
172.10	113.0
173.00	617.0
174.00	80256.0
175.00	5911.0
176.00	78712.0
177.00	4939.0
177.90	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012